





Current Data Parameters
NAME 1028-5023
EXPNO 1
PROCNO 1

F2 Acquisition Parameters

Date_ 20241020
Time 10.50
INSTRUM spect
PROBHD z116098_0490
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 MHz
FIDRES 0.244532 Hz
AQ 4.0894455 sec
RG 87.996
DW 62.400 usec
DE 6.50 usec
TE 298.0 K
D1 1.00000000 sec
TDC
SFO1 400.1524709 MHz
NUC1 1H
PC 10.00 usec
PLW1 14.69799999 W

F2 - Processing parameters

SI 65536
SF 400.1500011 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB
PC 1.00

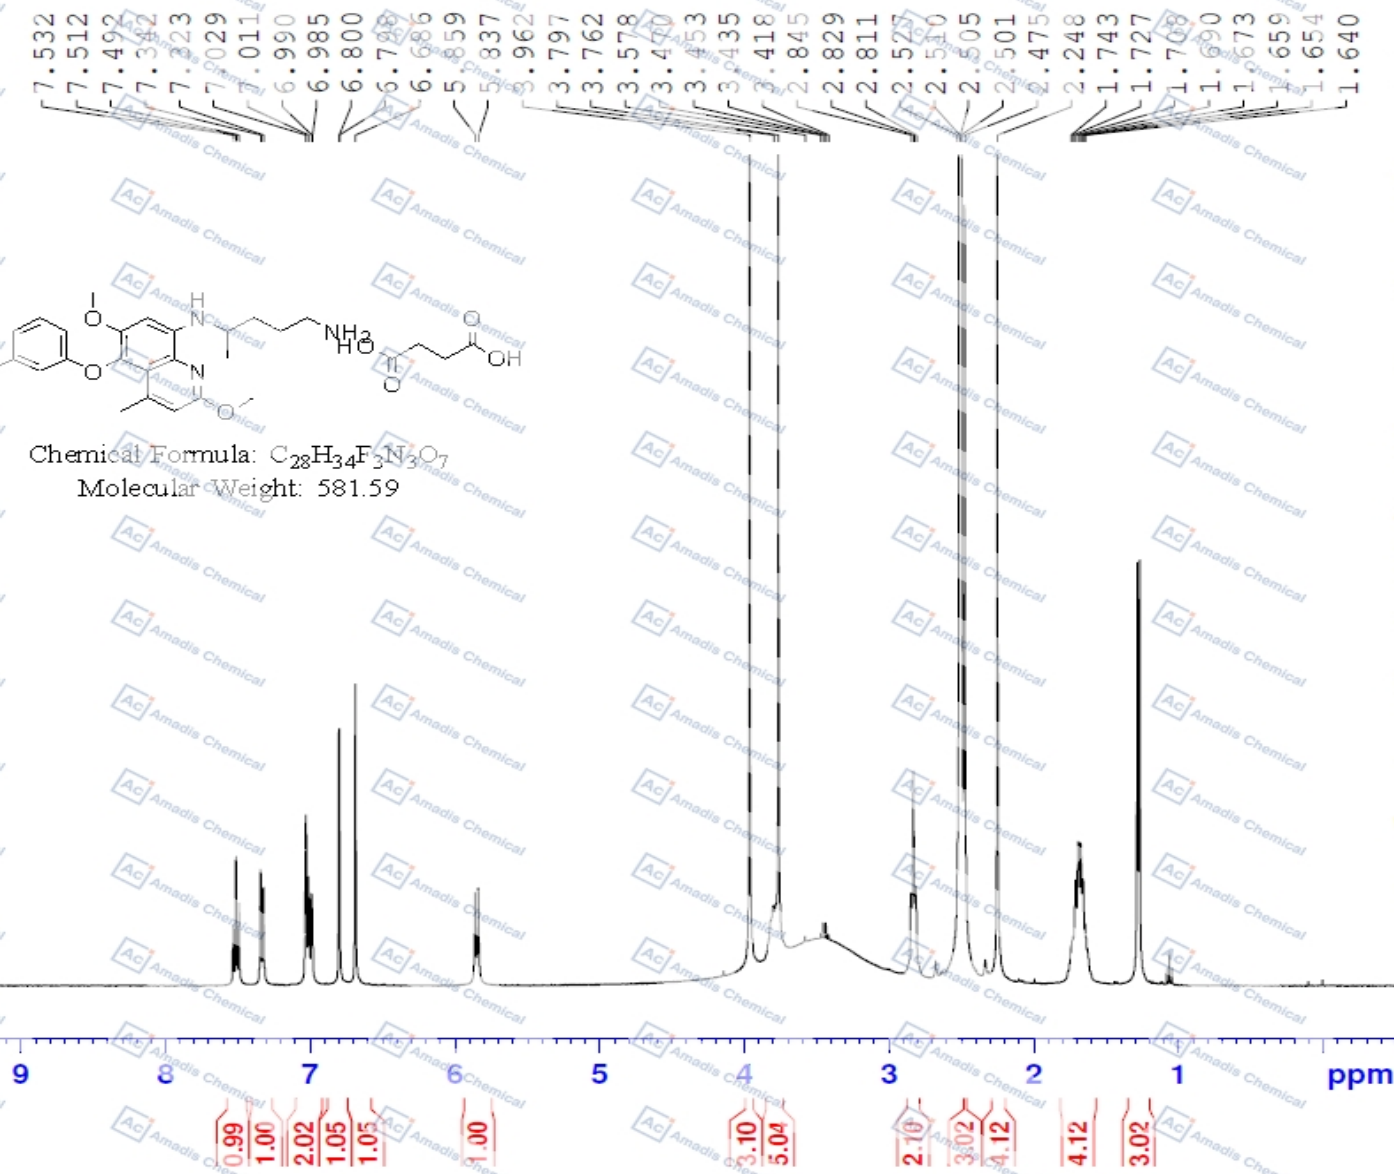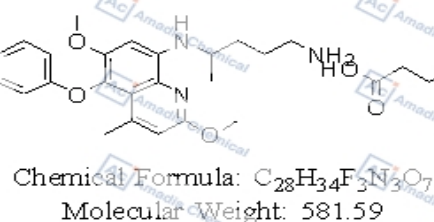

*For laboratory or manufacturing use only, not for drug, food and household use.