


MS of 117399-94-7

MASS SPECTROMETRY REPORT

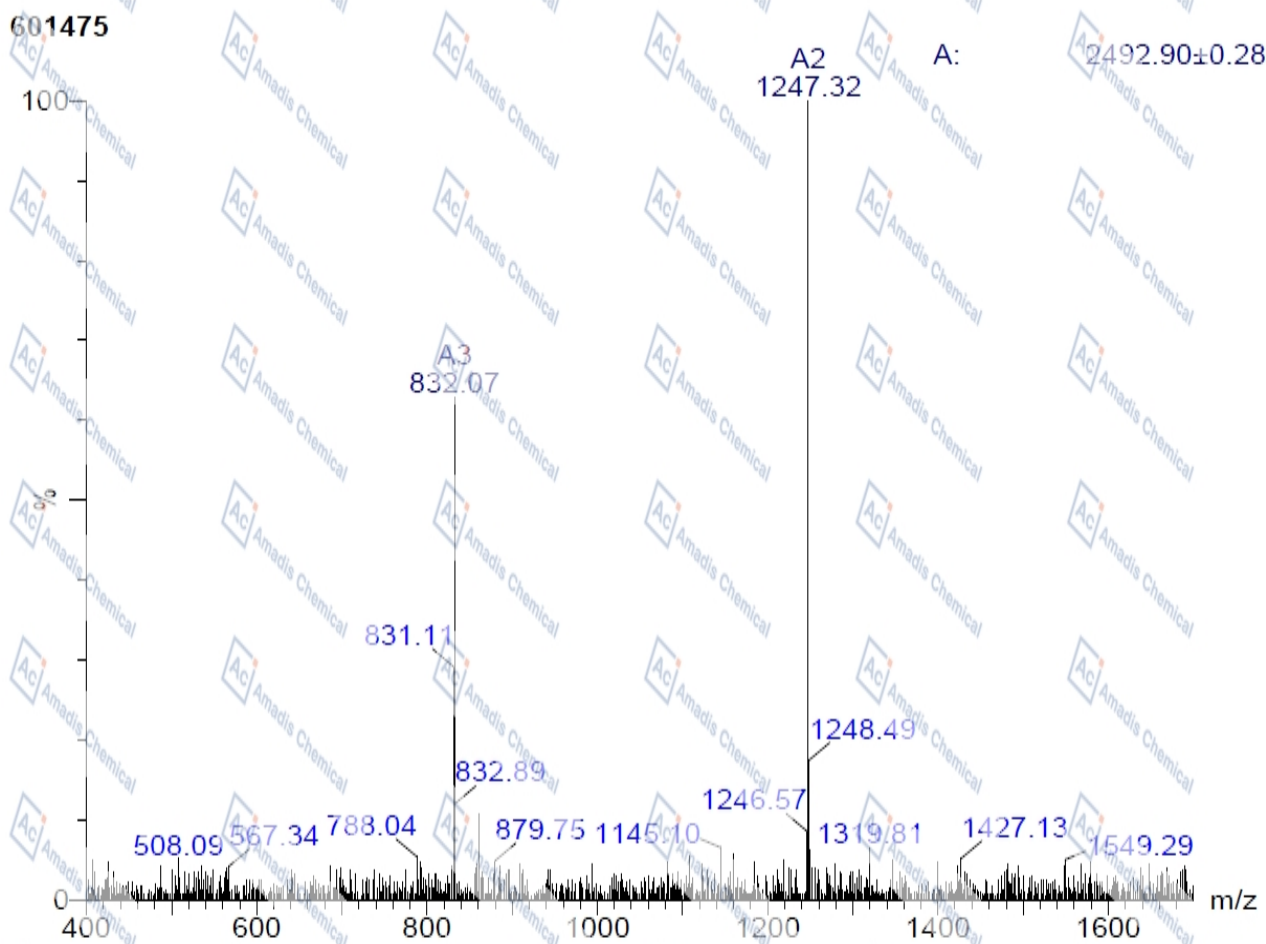

Sample Description

Analyzed date: 2024-06-14
 Analyst: SHAO
 Sample: 601475
 M.W.: 2491.9
 Lot No.:

Instrument

Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: 20.0v
 CDL Temp.: 250 °C
 Block Temp.: 200 °C

Waters 2695

Probe Bias: 4.5kv
 Detector: 1.5kV
 T. Flow: 0.5ml/min
 B. Conc.: 50%H₂O/50%ACN

***For laboratory or manufacturing use only, not for drug, food and household use.**

**if you have any comments and suggestions, please contact us by sales@amadischem.com*