


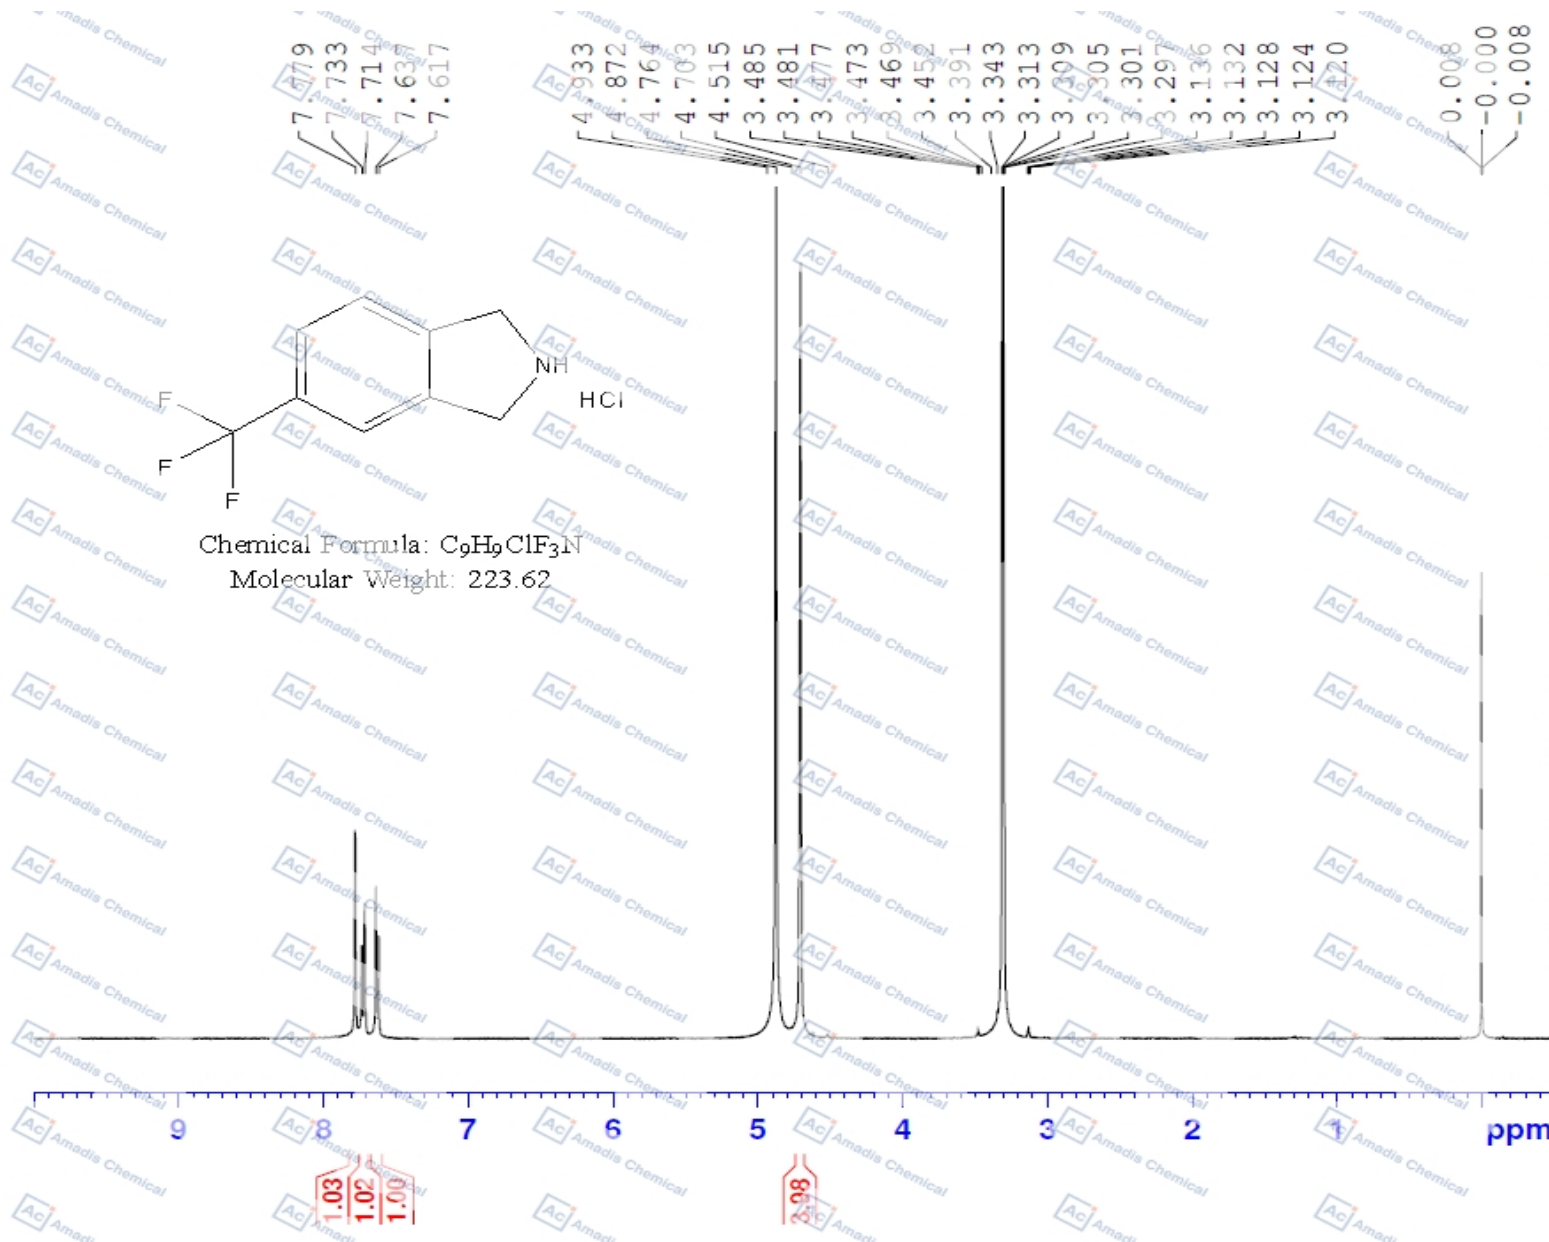

Current Data Parameters

NAME 1002-5107
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters

Date_ 20250103
Time 14:42 h
INSTRUM spect
PROBHD 7116098_0490 (zg30)
PULPROG zg30
TD 65536
SOLVENT MeOD
NS 16
DS 2
SWH 8012.879 Hz
FIDRES 0.244536 Hz
AQ 4.0894465 sec
RG 157.99
DW 62.400 usec
DE 6.500 usec
TE 295.8 K
D1 1.0000000 sec
TD0 1
SFO 400.152470 MHz
NUC1 1H
P1 10.00 usec
PIV 15.59300041 W

F2 - Processing parameters

SI 65536
SF 400.150097 MHz
WDW 0
SSB 0
LB 0.30 Hz
GB 0
PC 1

*For laboratory or manufacturing use only, not for drug, food and household use.