



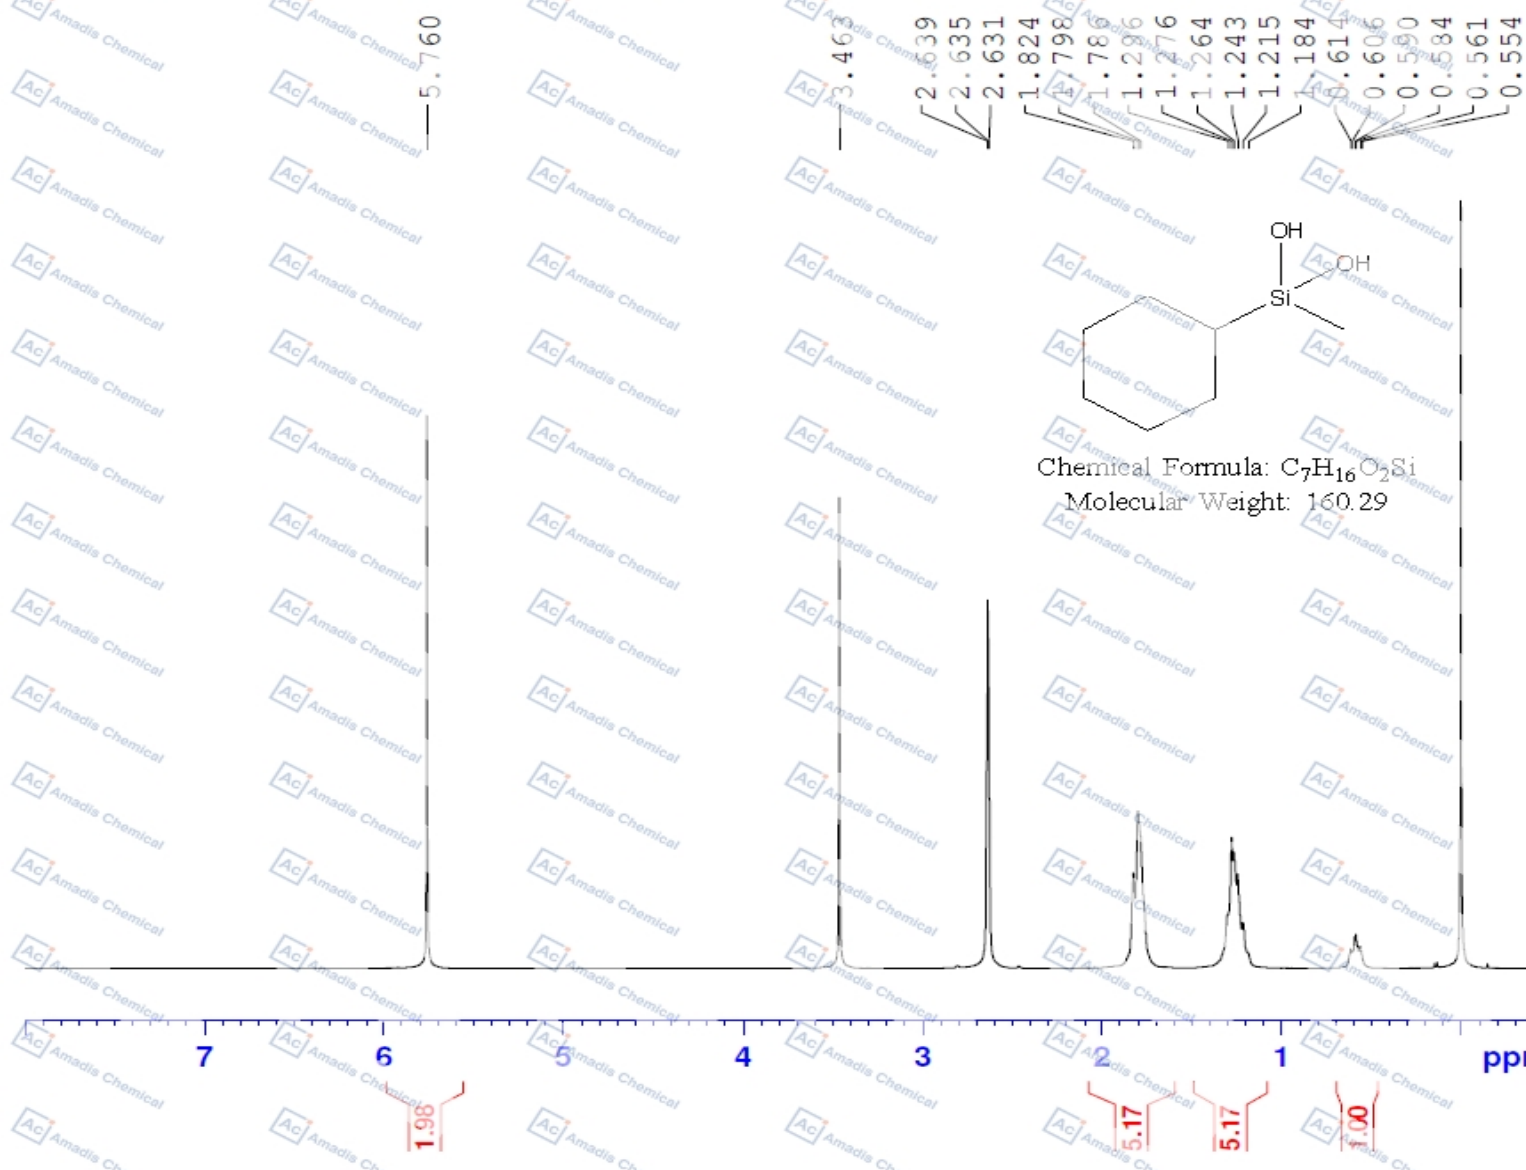

Current Data Parameters
NAME 1106-5043
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20241107
Time 15:41 h
INSTRUM spect
PROBHD 116098_0490 (1H)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 67.79
IN 62.4600 usec
DE 6.50 usec
TE 298.0 K
D1 1.0000000 sec
T0 1
SFO1 400.1524700 MHz
NUC1 1H
P1 10.00 usec
PRW1 14.6979995 W

F2 - Processing parameters
SI 65536
SF 400.1499997 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

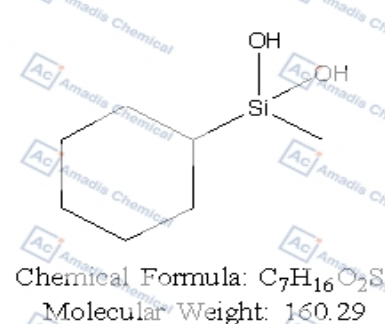

*For laboratory or manufacturing use only, not for drug, food and household use.