


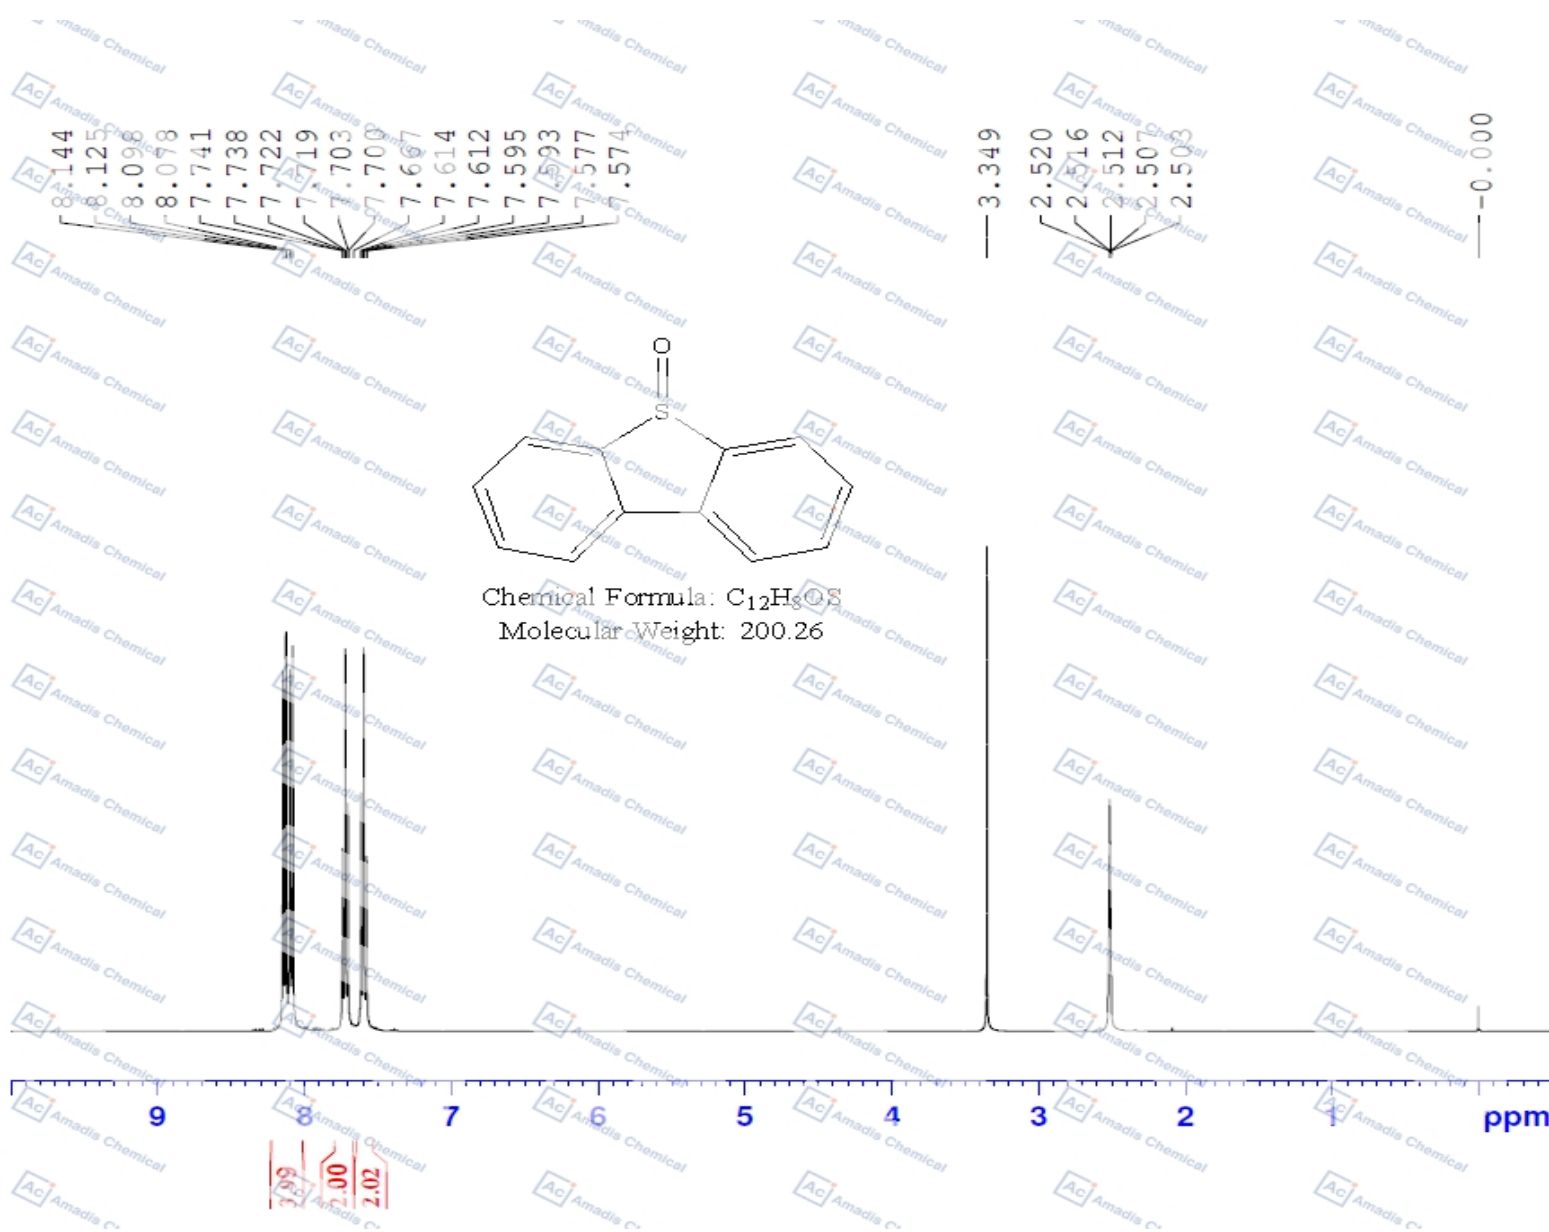

Current Data Parameters
NAME 0516-5292
EXPNO 10
PROCNO

F2 - Acquisition Parameters

Date 20250516
Time 11:30 h
INSTRUM spect
PROBHD 116098_0490 (z30)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 87.96
DW 62.400 usec
DE 6.50 usec
TE 298.8 K
D1 1.0000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PLW1 15.59300001 W

F2 - Processing parameters

SI 65536
SF 400.1499981 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.