



Current Data Parameters
NAME 0812-4920
EXPNO 10
PROCNO 1



F2 - Acquisition Parameters

Date_ 20240813
Time 14:02 h
INSTRUM spect
PROBHD 116098_0490 (zgc30)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.840 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 123.07
DW 62.400 usec
DE 6.50 usec
TE 298.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 14.69799395 W

F2 - Processing parameters

SI 65536
SF 400.150026 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.60

10.322

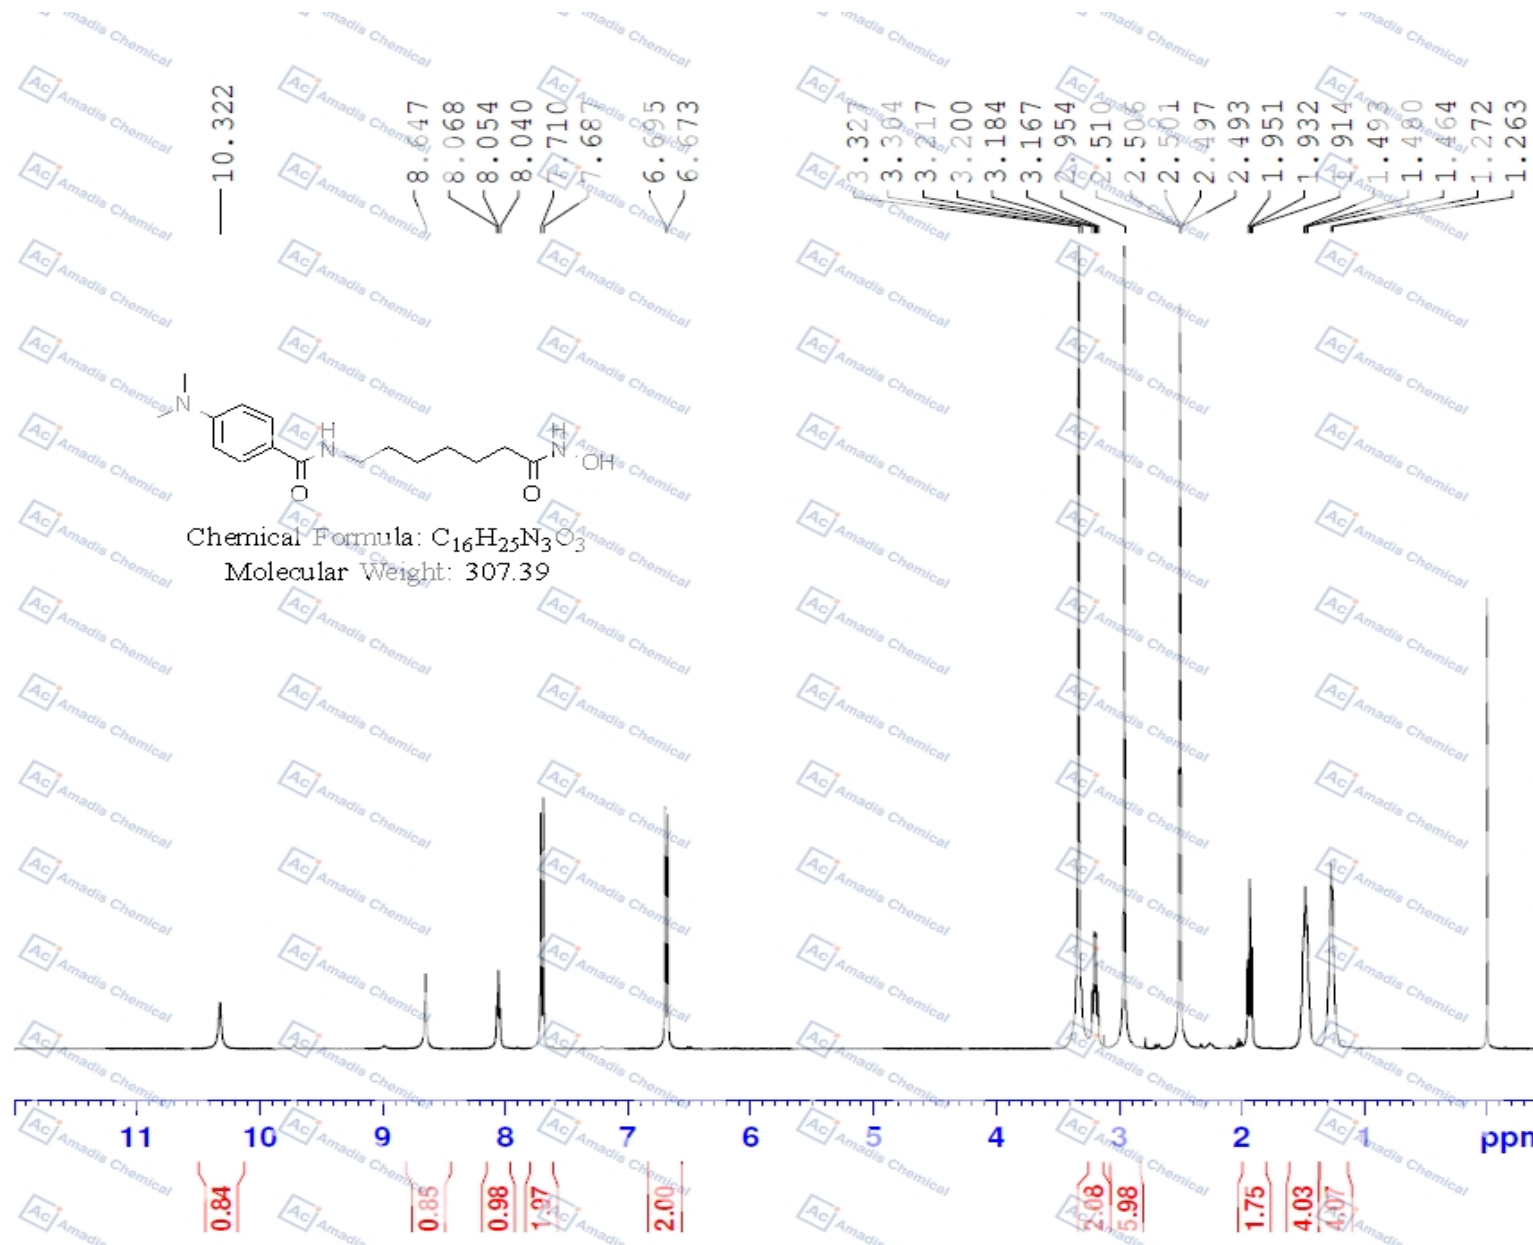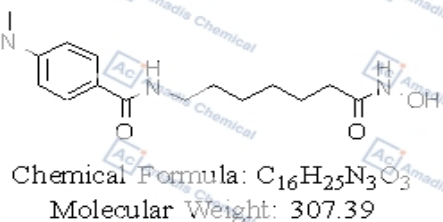

*For laboratory or manufacturing use only, not for drug, food and household use.