


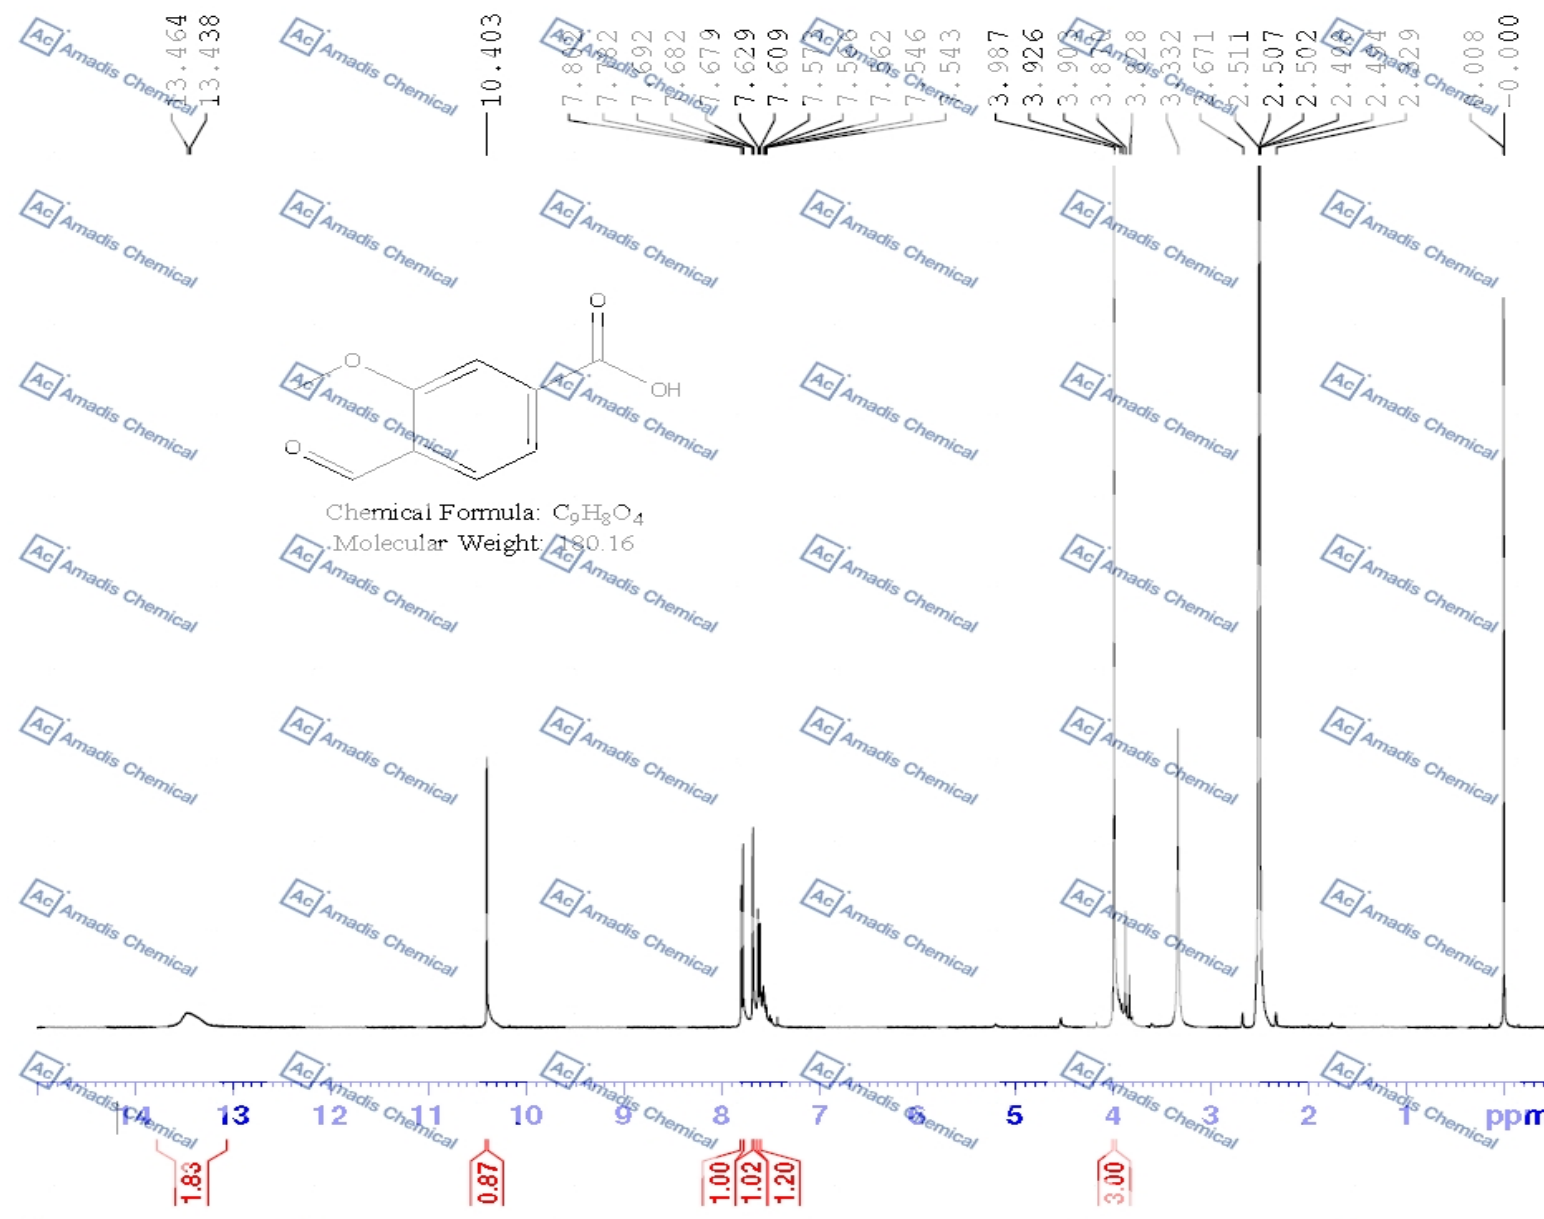

BRUKER

Current Data Parameters
NAME 0306-4647
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240307
Time_ 14.11h
INSTRUM spect
PROBHD zg30
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244726 Hz
AQ 4.089466 sec
RG 157.99
DW 62.400 usec
DE 6.50 usec
TE 295.3 K
D1 1.00000000 sec
TDO 1
SFO 400.152470 MHz
NUC1 13C
P1 10.00 usec
PLW1 14.69799995 W

F2 - Processing parameters
SI 65536
SF 400.150022 MHz
WDW EM
SS 0
LB 0.30 Hz
GB
PC 1.00

*For R&D use only