



Current Data Parameters


NAME 1011-5001
EXPNO 1.0
PROCNO 1

F2 - Acquisition Parameters

Date_ 20241012
Time 11.41
INSTRUM spect
PROBHD Z116098_0480 (4g)
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.089465 sec
RG 79.19
DW 62.400 usec
DE 6.50 usec
TE 298.5 K
D1 1.0000000 sec
TD0
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 14.69799995 W

F2 - Processing parameters

SI 32768
SF 400.1500082 MHz
WDW EM
SSB 0
LB 30 Hz
GB 0
PC 1.00

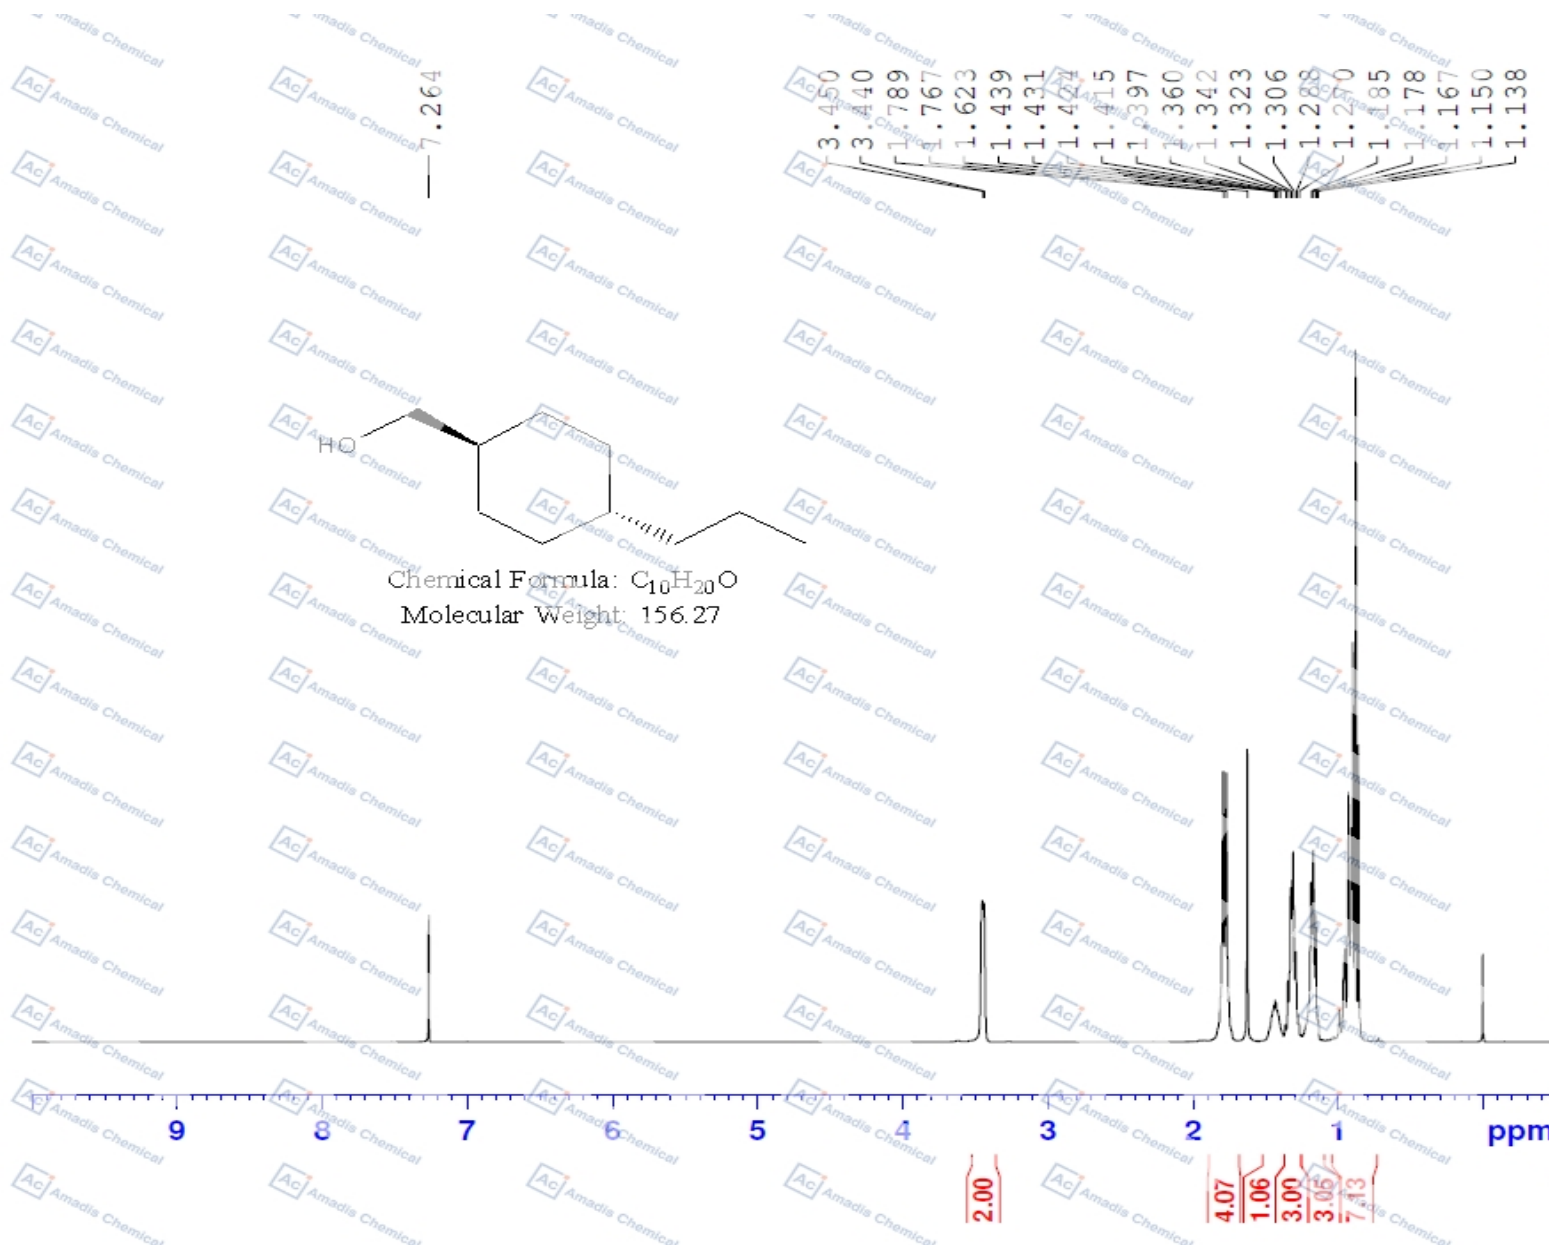

*For laboratory or manufacturing use only, not for drug, food and household use.