


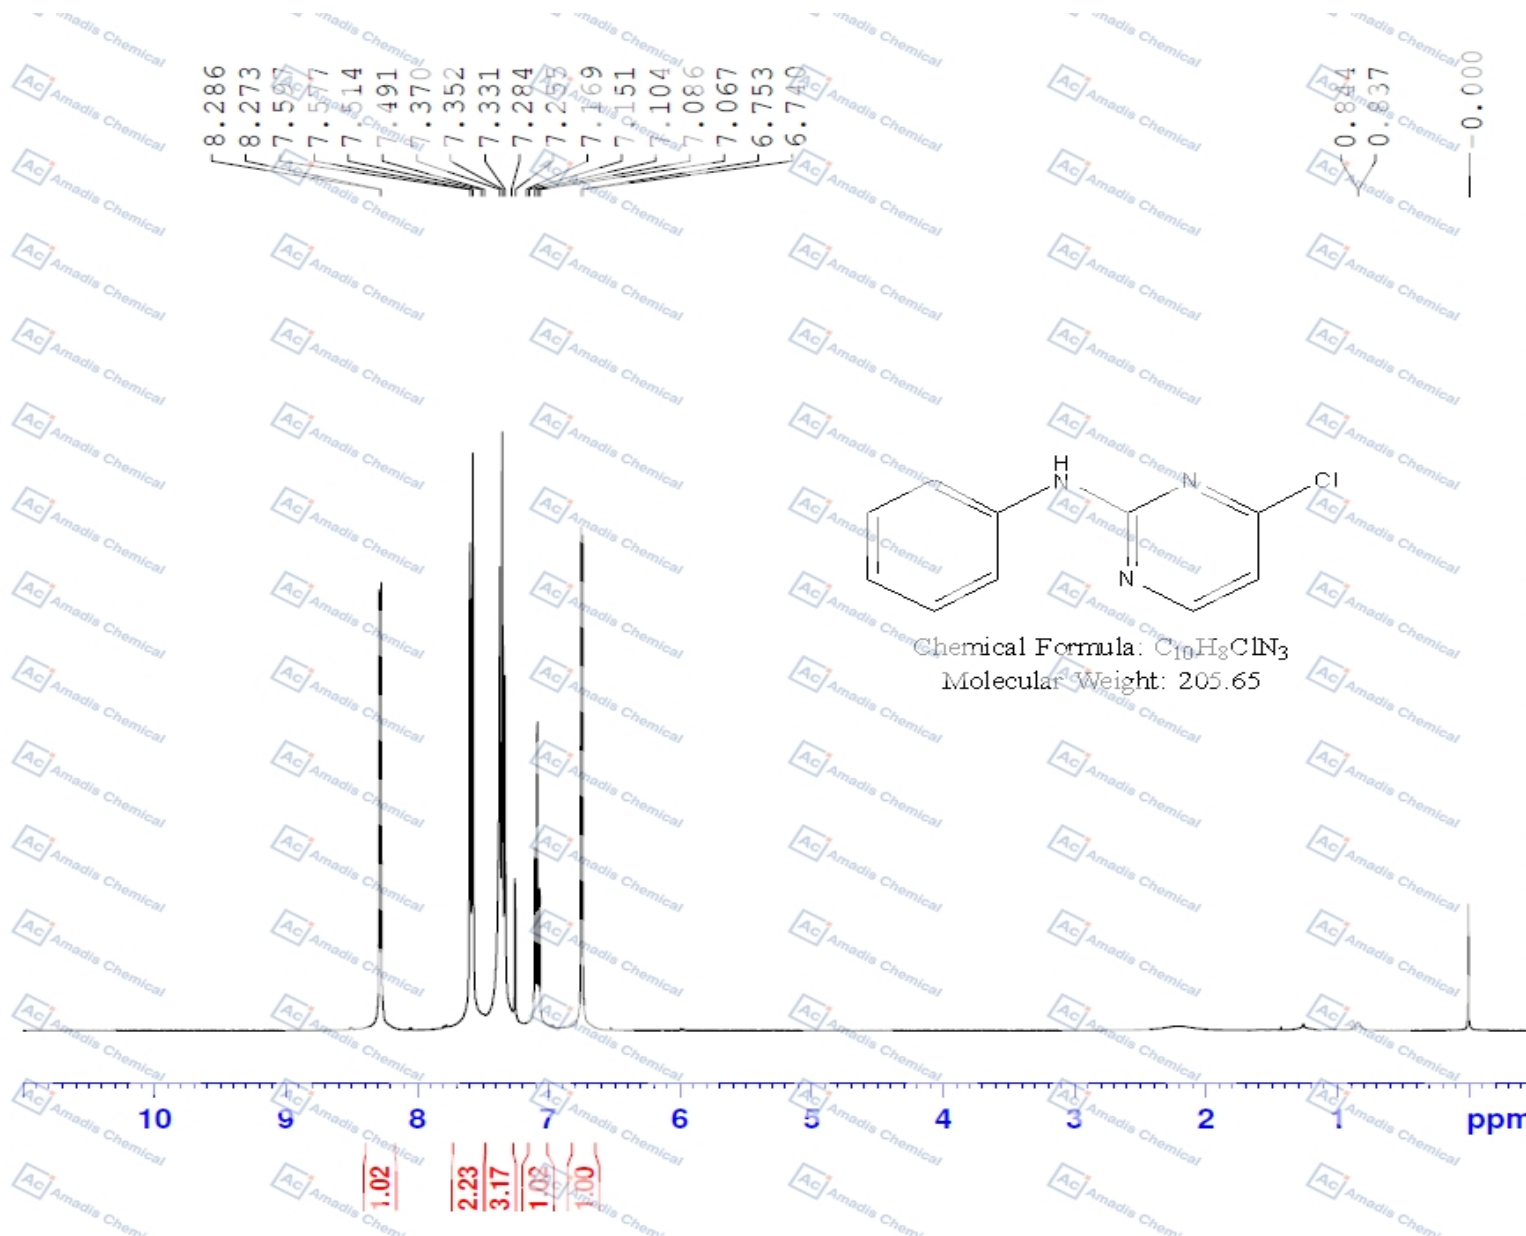

Current Data Parameters
NAME 0809-4916
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters

Date_ 20240816
Time 12.29
INSTRUM spect
PROBHD z116098_0490 (1H/13C)
PULPROG zgpg30
TD 65536
SOLVENT CDCl₃
NS 16
DS 2
SWH 8012.820 MHz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 98.83
DW 62.460 usec
DE 6.50 usec
TE 298.1 K
D1 1.00000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 14.69799928 W

F2 - Processing parameters

SI 65536
SF 400.1500178 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.