


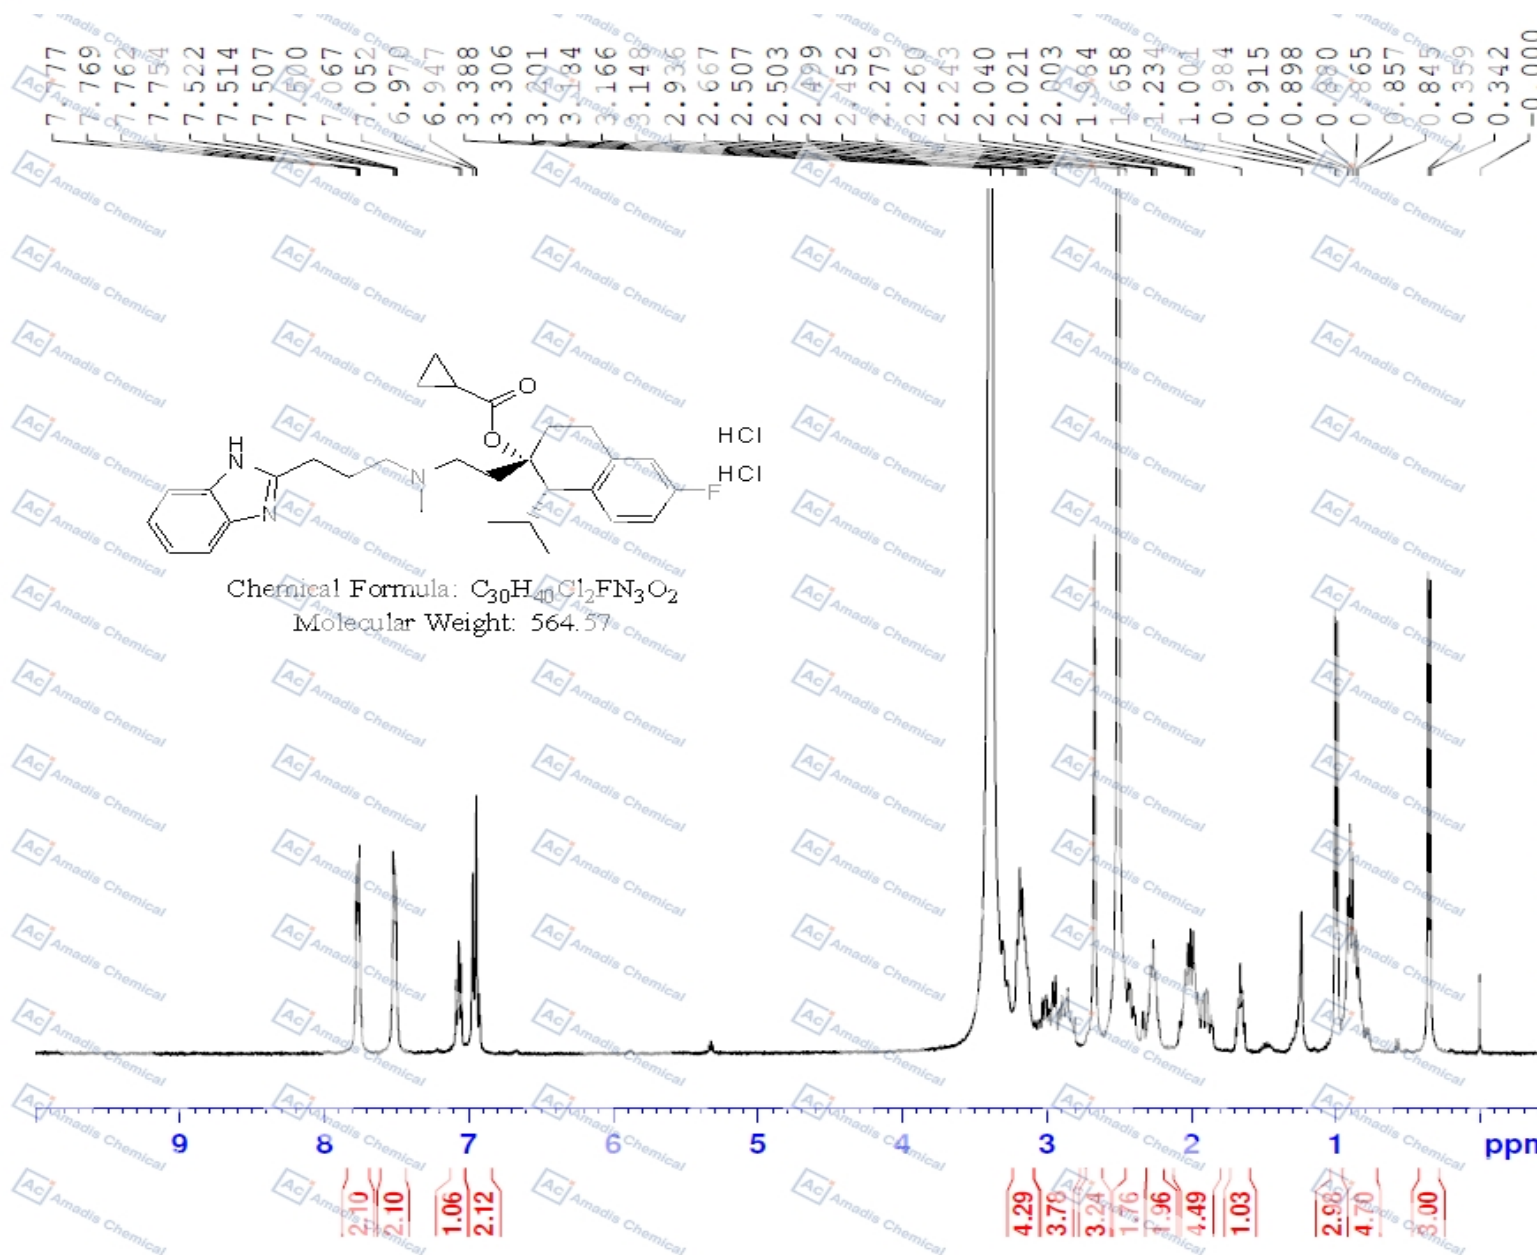

Current Data Parameters

NAME 0304-546
EXPNO 1
PROCNO 1

F2 Acquisition Parameters

Date_ 20250309
Time 11:58 H
INSTRUM spect
PROBHD Z116098_0490
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 6
DS 4
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.089465 sec
RG 123.07
DW 62.400 usec
DE 6.50 usec
TE 295.2 K
D1 1.00000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PLW1 15.59300041 W

F2 Processing parameters

SI 65536
SF 400.1500020 MHz
WDW EM
SSB 0
LB 0.430 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.