




Current Data Parameters
NAME 0522-4778
EXPNO 20
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240523
Time 15.32 h
INSTRUM spect
PROBHD Z116098_0490
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.08944 sec
RG 111.92
DW 62.400 usec
DE 6.50 usec
TE 298.8 K
D1 1.00000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC 1H
P1 10.00 usec
PLW1 14.69799995 W

F2 - Processing parameters
SI 65536
SF 400.1500026 MHz
WDW EM
SSB 0
LB 0.0 Hz
GB 0
PC 1.00

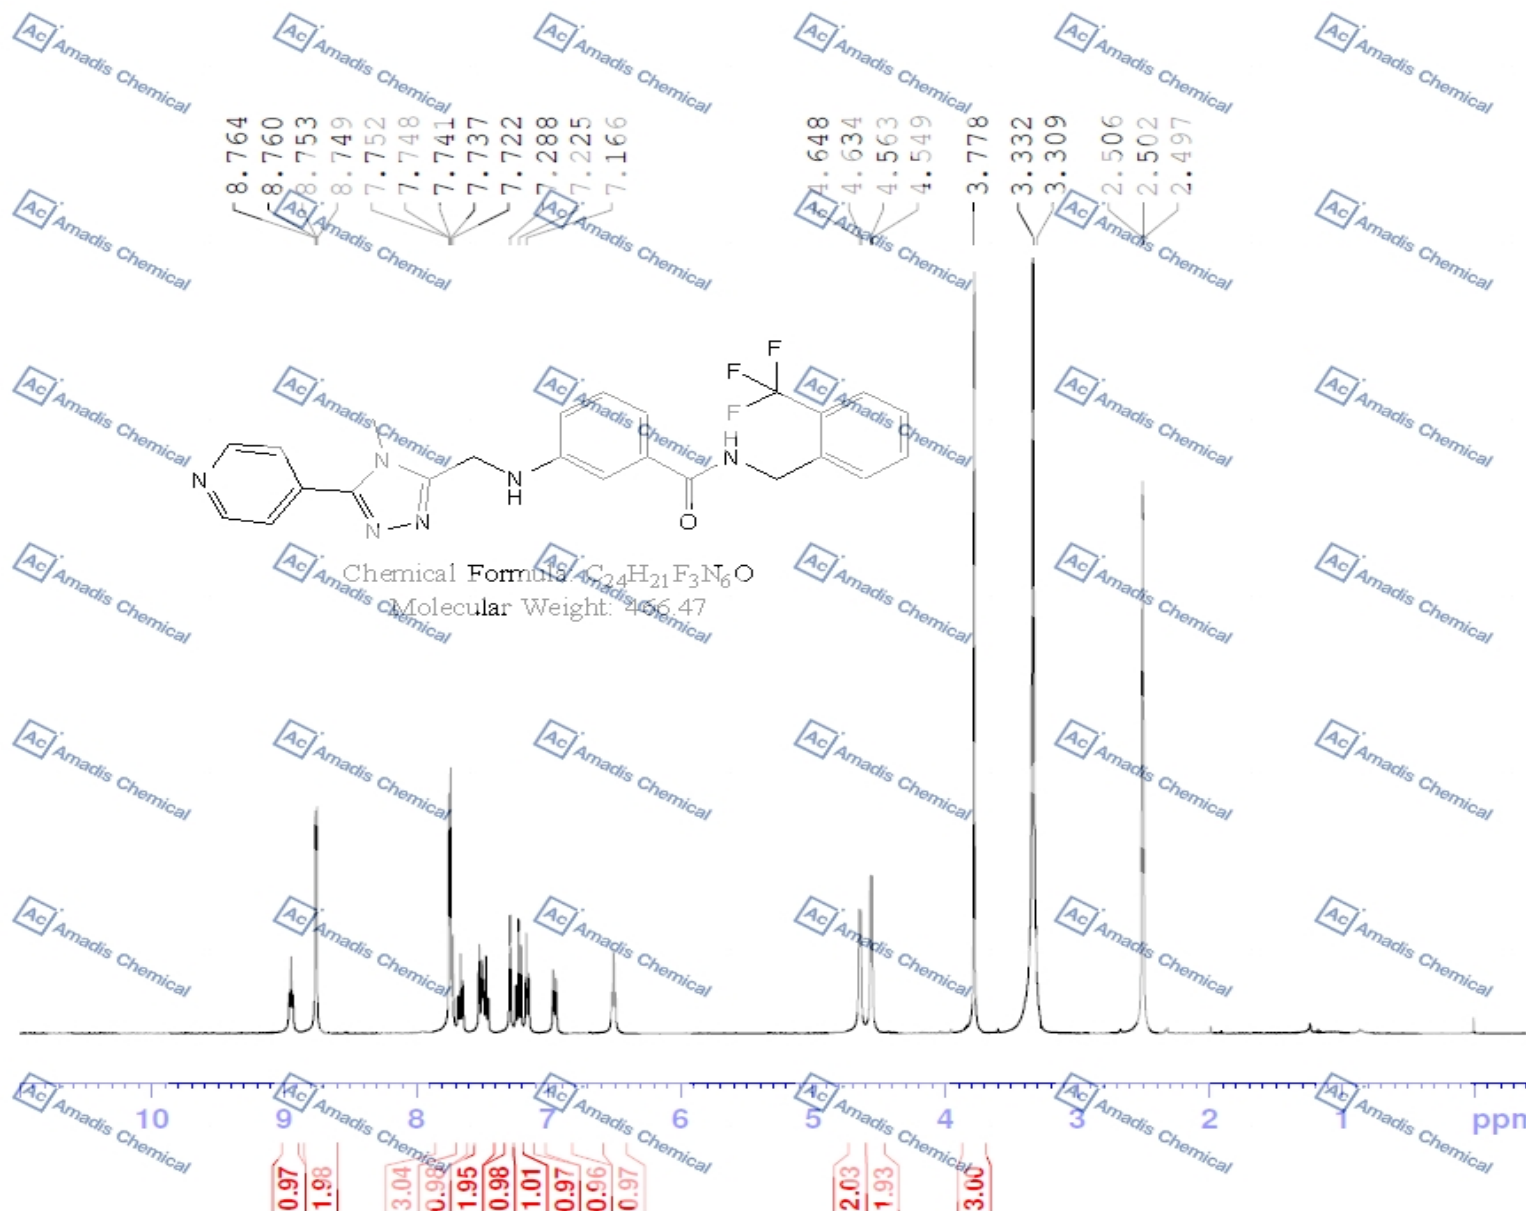

*For laboratory or manufacturing use only, not for drug, food and household use.