


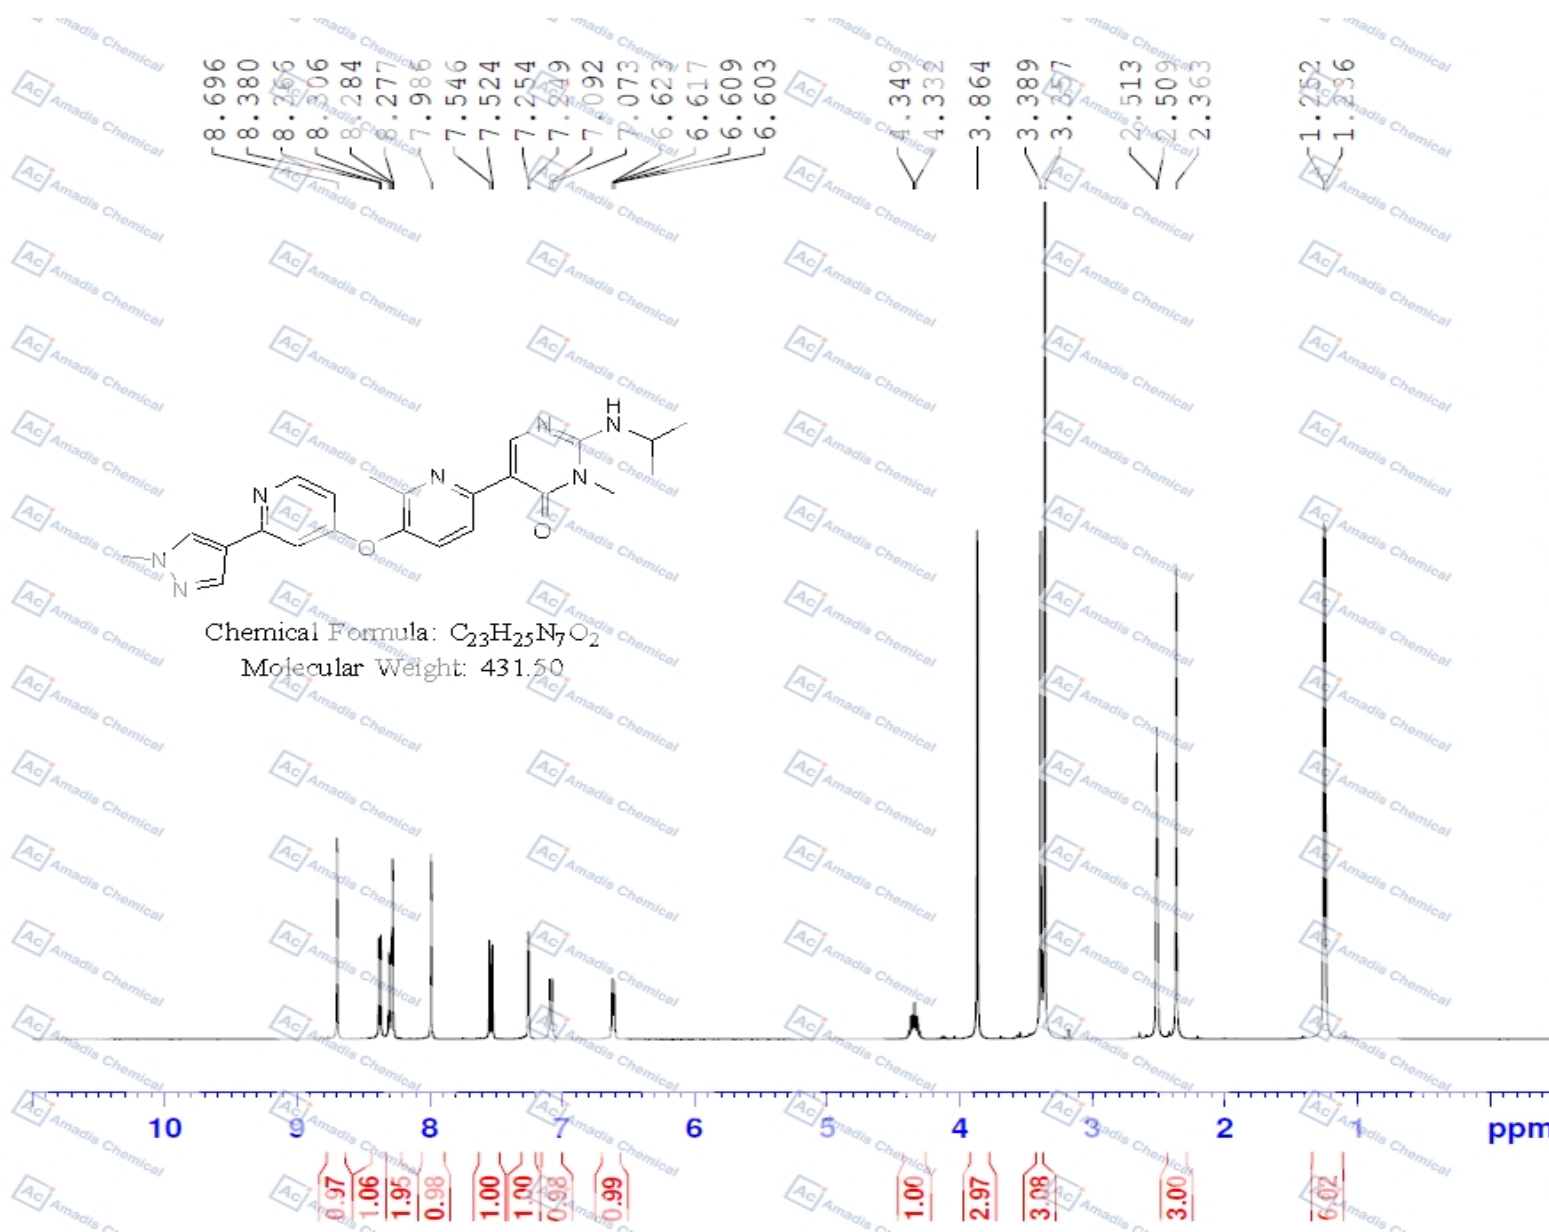

Current Data Parameters
NAME 0221-5159
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250225
Time 18:56 h
INSTRUM spect
PROBHD 116098_0490 (400 MHz)
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.920 Hz
FIDRES 0.244537 Hz
AQ 4.0894465 sec
RG 87.96
SF 624.00 usec
DE 6.50 usec
TE 295.0 K
D1 1.0000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 15.5930041 W

F2 - Processing parameters
SI 65536
CF 400.150000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.