
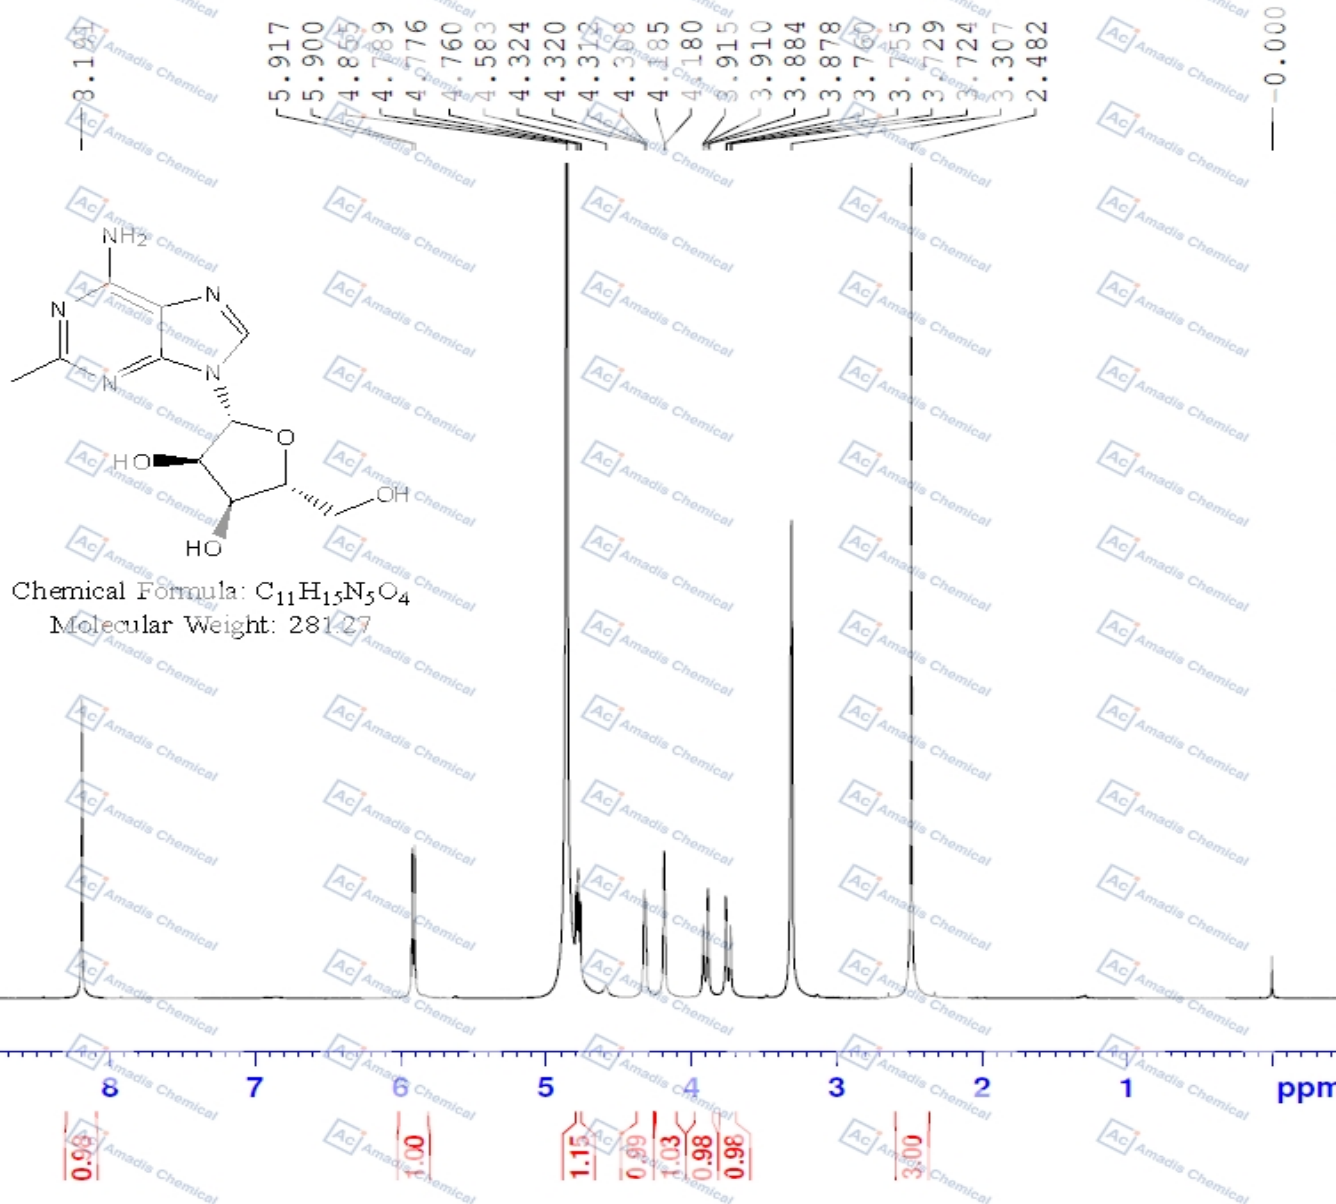


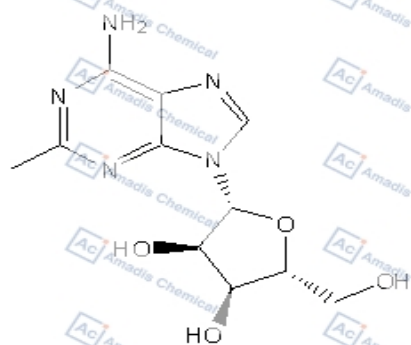

Current Data Parameters
NAME 1010-4996
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters

Date_ 20240714
Time 11.15
INSTRUM spect
PROBHD Z116098_0490 (400 MHz)
PULPROG zgpg30
TD 65536
SOLVENT MeOD
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894165 sec
RG 114.92
DW 62.400 usec
DE 6.50 usec
TE 298.5 K
D1 1.00000000 sec
TDO
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PLN1 14.69799995 W

F2 - Processing parameters

SI 32768
SF 400.1500000 MHz
WDW EM
SSB 0
LA 30 Hz
GB
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.