


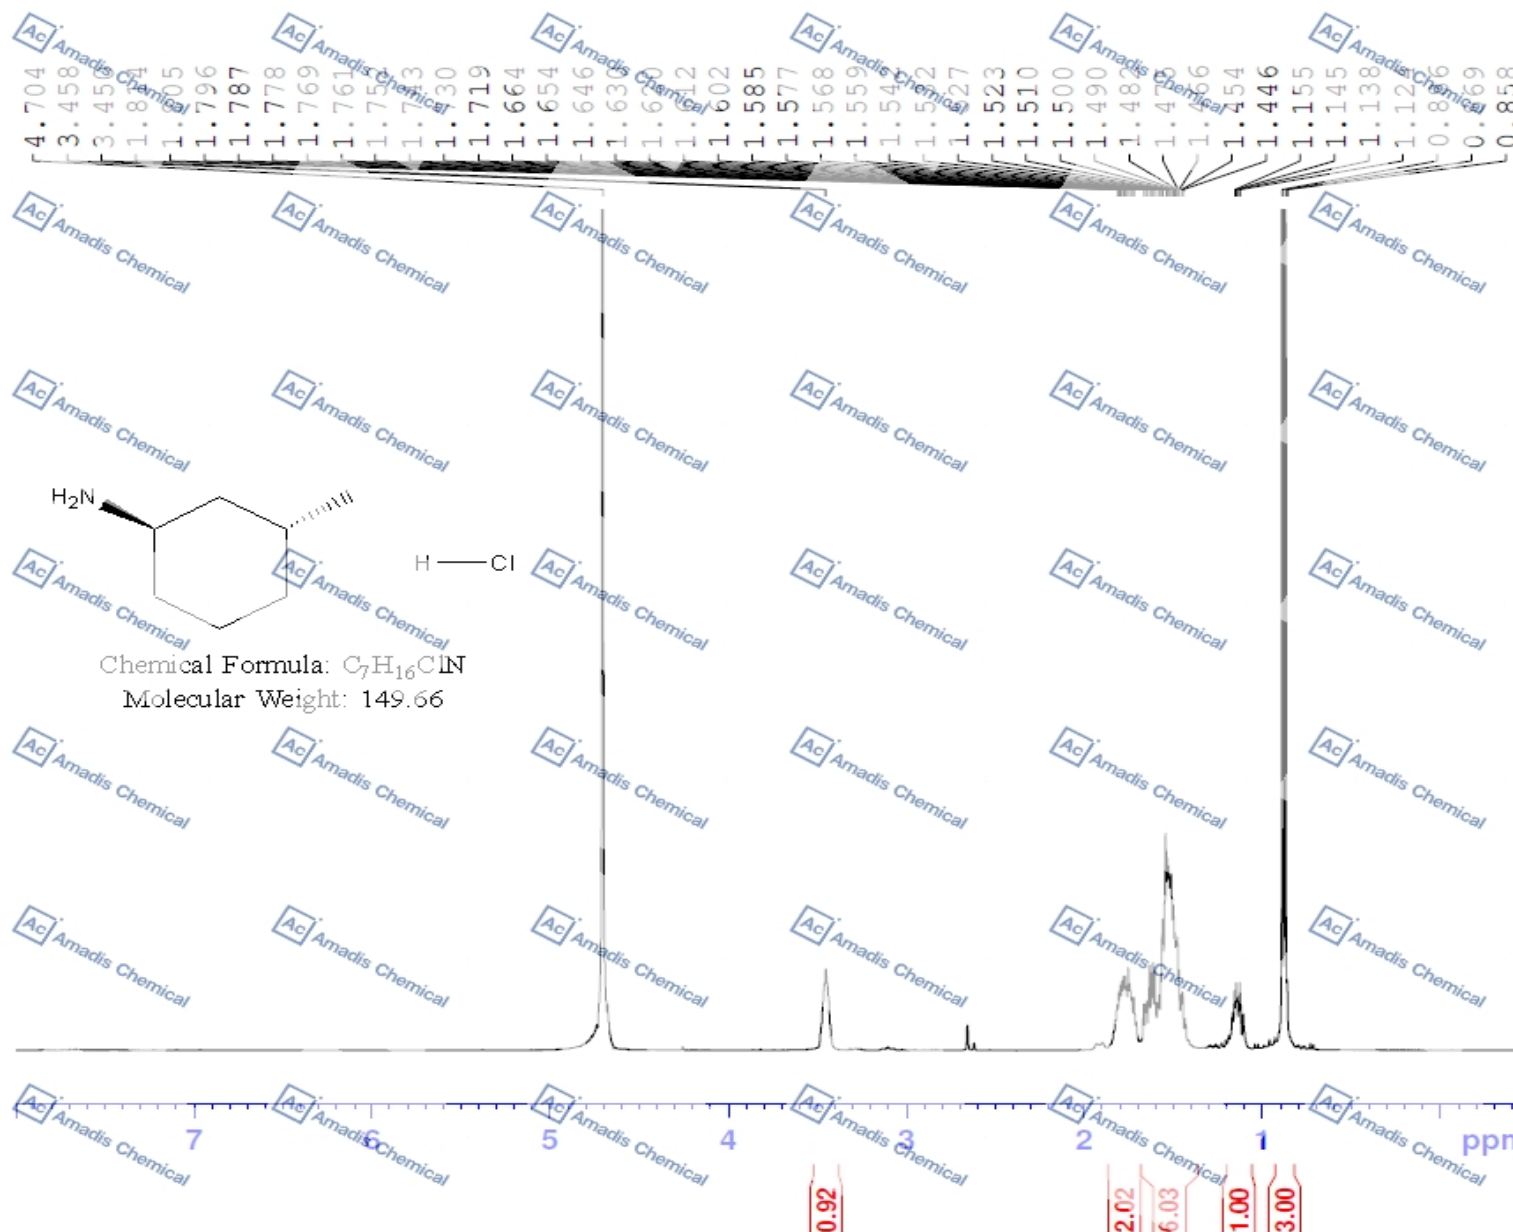

**BRUKER**

Current Data Parameters  
NAME 0705-4873  
EXPNO 10  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20240708  
Time\_ 13.32 h  
INS\_ spect  
PROB\_ zg30  
PULPROG\_ 65536  
TD\_ 65536  
SOLVENT\_ D2O  
NS\_ 16  
DS\_ 2  
SWH\_ 8012.820 Hz  
FIDRES\_ 0.244538 Hz  
AQ\_ 4.08944 sec  
RG\_ 67.79  
DW\_ 62.400 usec  
DE\_ 6.50 usec  
TE\_ 299.4 K  
D1\_ 1.0000000 sec  
TD0\_ 1  
SFO1\_ 400.1524709 MHz  
NUC1\_ 1H  
P1\_ 10.00 usec  
PLW1\_ 14.69799995 W

F2 - Processing parameters  
SI\_ 65536  
SF\_ 400.1500000 MHz  
WDW\_ EM  
SSB\_ 0  
LB\_ 0.00 Hz  
GB\_ 0  
PC\_ 1.00

\*For laboratory or manufacturing use only, not for drug, food and household use.