


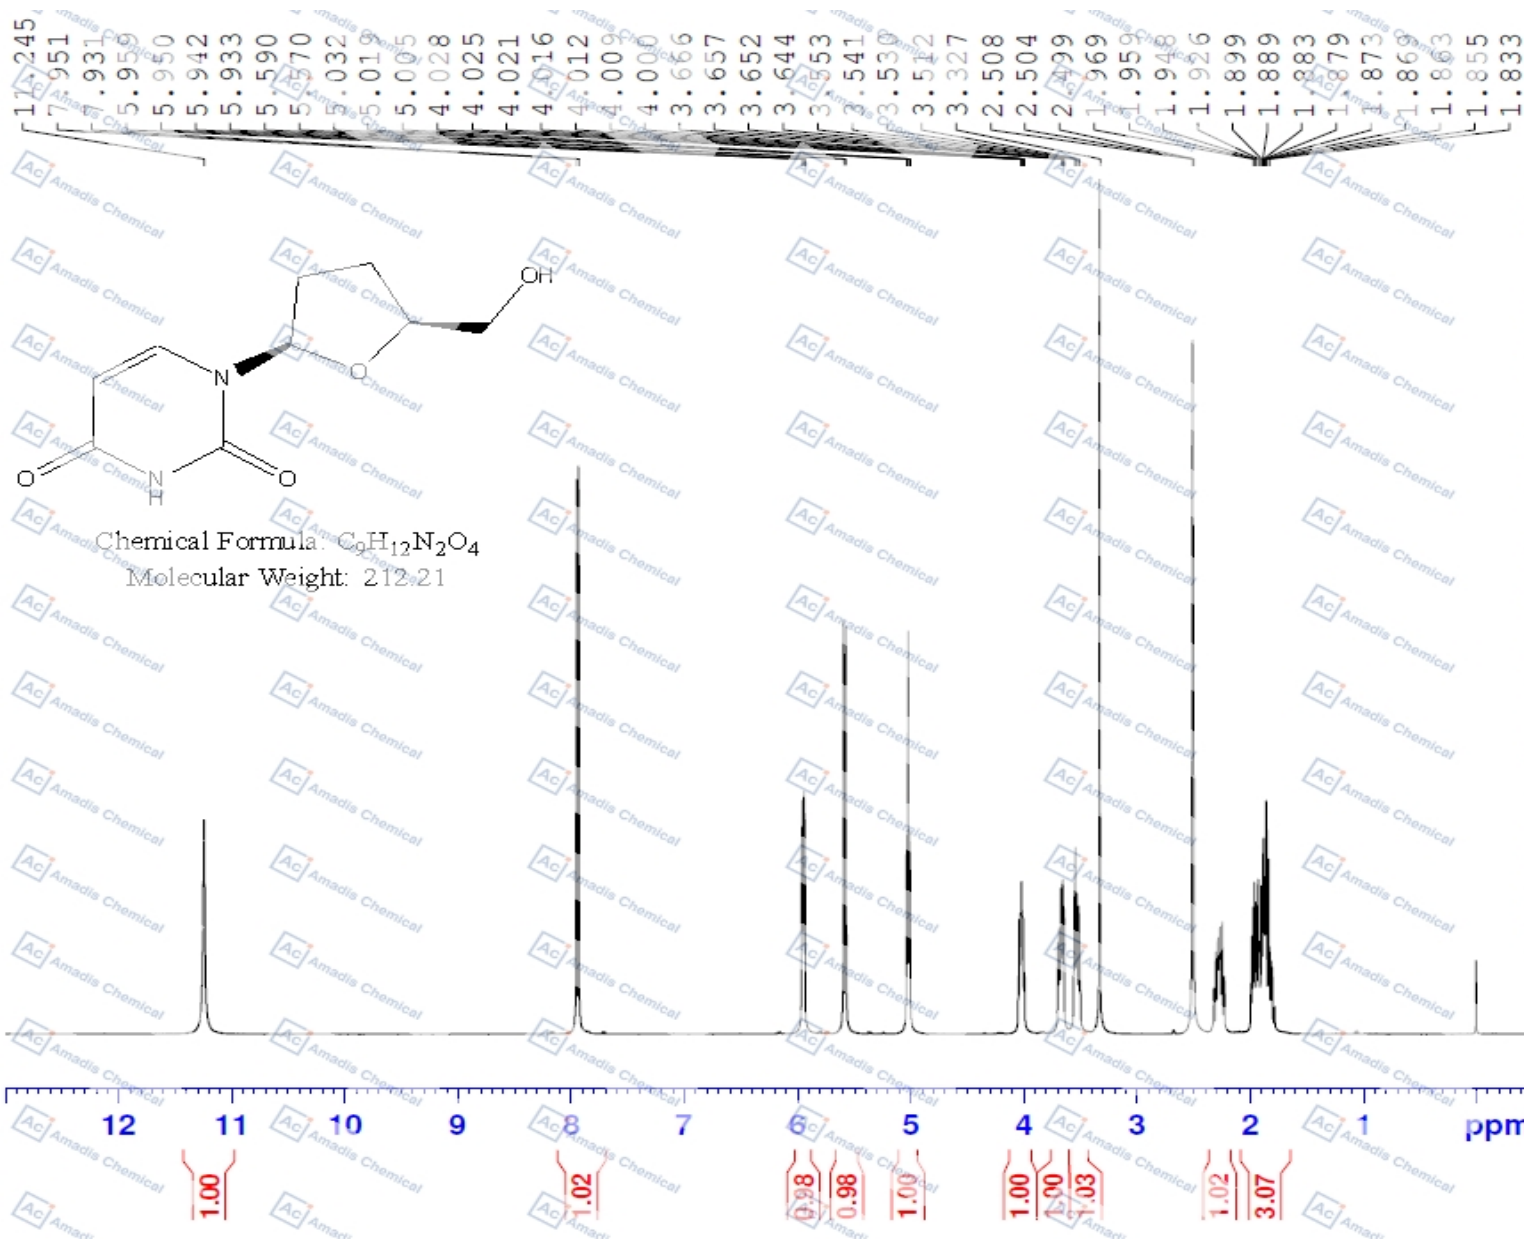

BRUKER

Current Data Parameters	
NAME	0516-5289
EXPNO	10
PROCNO	1

F2 - Acquisition Parameters	
Date_	20250516
Time	11:27 h
INSTRUM	spec
PROBHD	Z116098_0490 (
PULPROG	zg30
TD	65536
SOLVENT	DMSO
NS	16
DS	2
SWH	8012.920 Hz
FIDRES	0.244537 Hz
AQ	4.0894465 sec
RG	87.96
DW	62.400 usec
DE	6.50 usec
TE	298.8 K
D1	1.00000000 sec
TD0	1
SECT	400.1524709 MHz
NUC1	1H
P1	10.00 usec
PLW1	15.59300041 W

F2 - Processing parameters	
SI	65536
SF	400.1500014 MHz
WDW	EM
SSB	0
LB	0.30 Hz
GB	0
PC	1.00

*For laboratory or manufacturing use only, not for drug, food and household use.