




Current Data Parameters
NAME 0819-4930
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240820
Time 11:40 h
INSTRUM spect
PROBHD 116098_0490 (1H/13C) BBO
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SFO1 8012.620 MHz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 79.19
DW 62.500 usec
DE 6.50 usec
TE 297.9 K
D1 1.0000000 sec
TDO 0
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 0
PT1 14.6979995 W

F2 - Processing parameters
SI 65536
SF 400.1501662 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

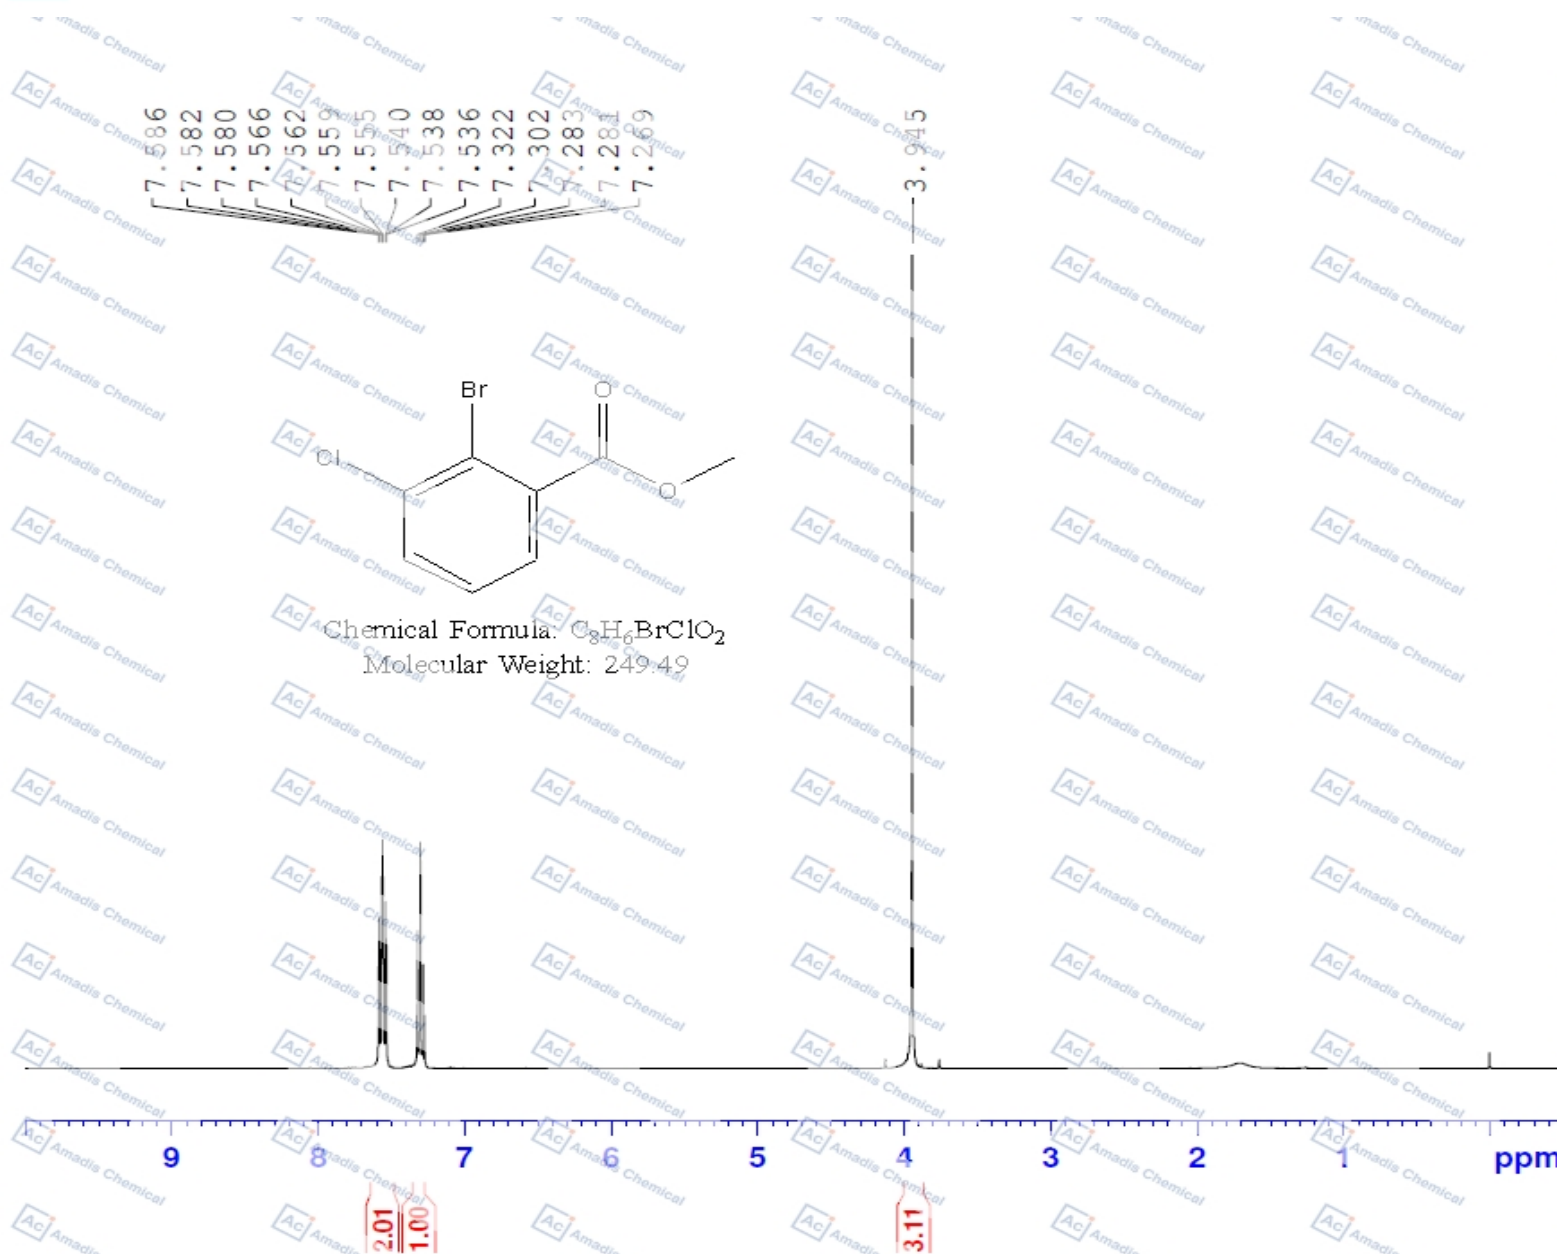

*For laboratory or manufacturing use only, not for drug, food and household use.