


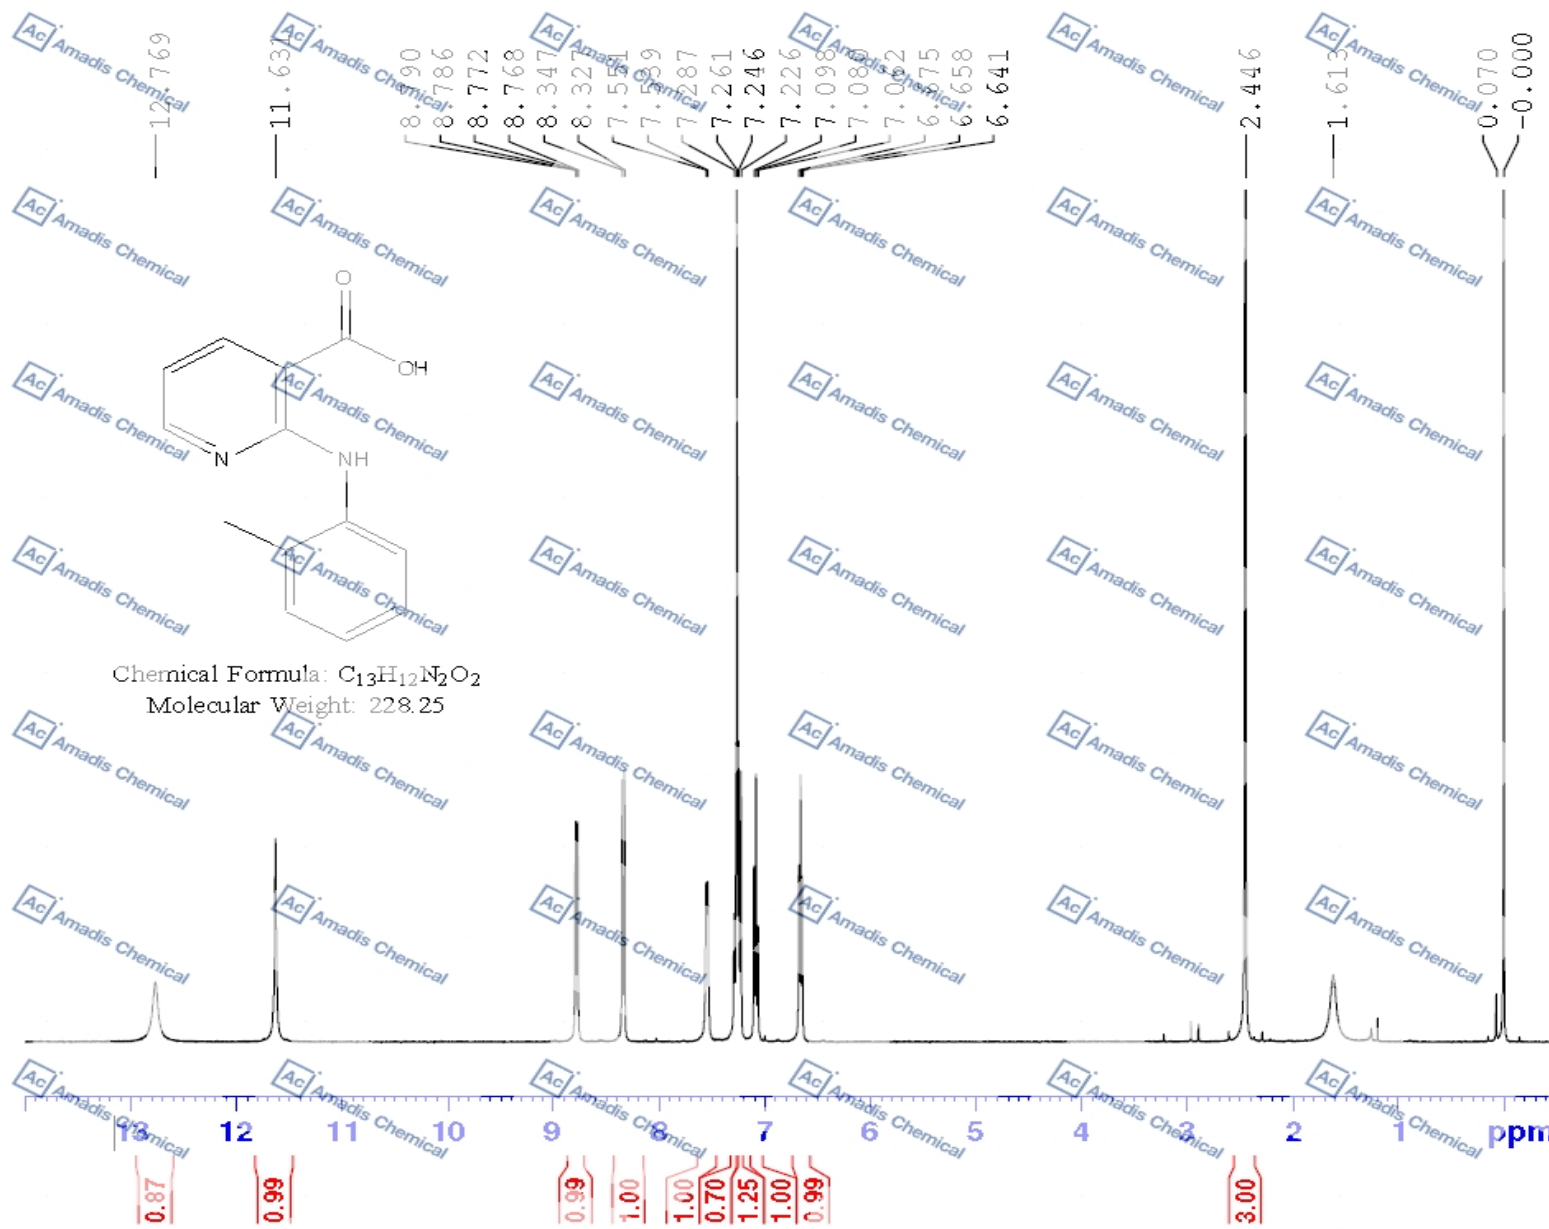

BRUKER

Current Data Parameters
NAME 0228-4637
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters

Date_ 20240229
Time 10:34 h
INSTRUM spect
PROBHD 2116098_0490
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.24432 Hz
AQ 4.0894765 sec
RG 157.99
DW 62.400 usec
DE 6.50 usec
TE 294.9 K
D1 1.00000000 sec
TD0 1
SF 400.152409 MHz
NUC1 1H
P1 10.00 usec
PLW1 14.6979995 W

F2 - Processing parameters

SI 65536
SF 400.150093 MHz
WDW EM
SFB 0
LB 0.3 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.