


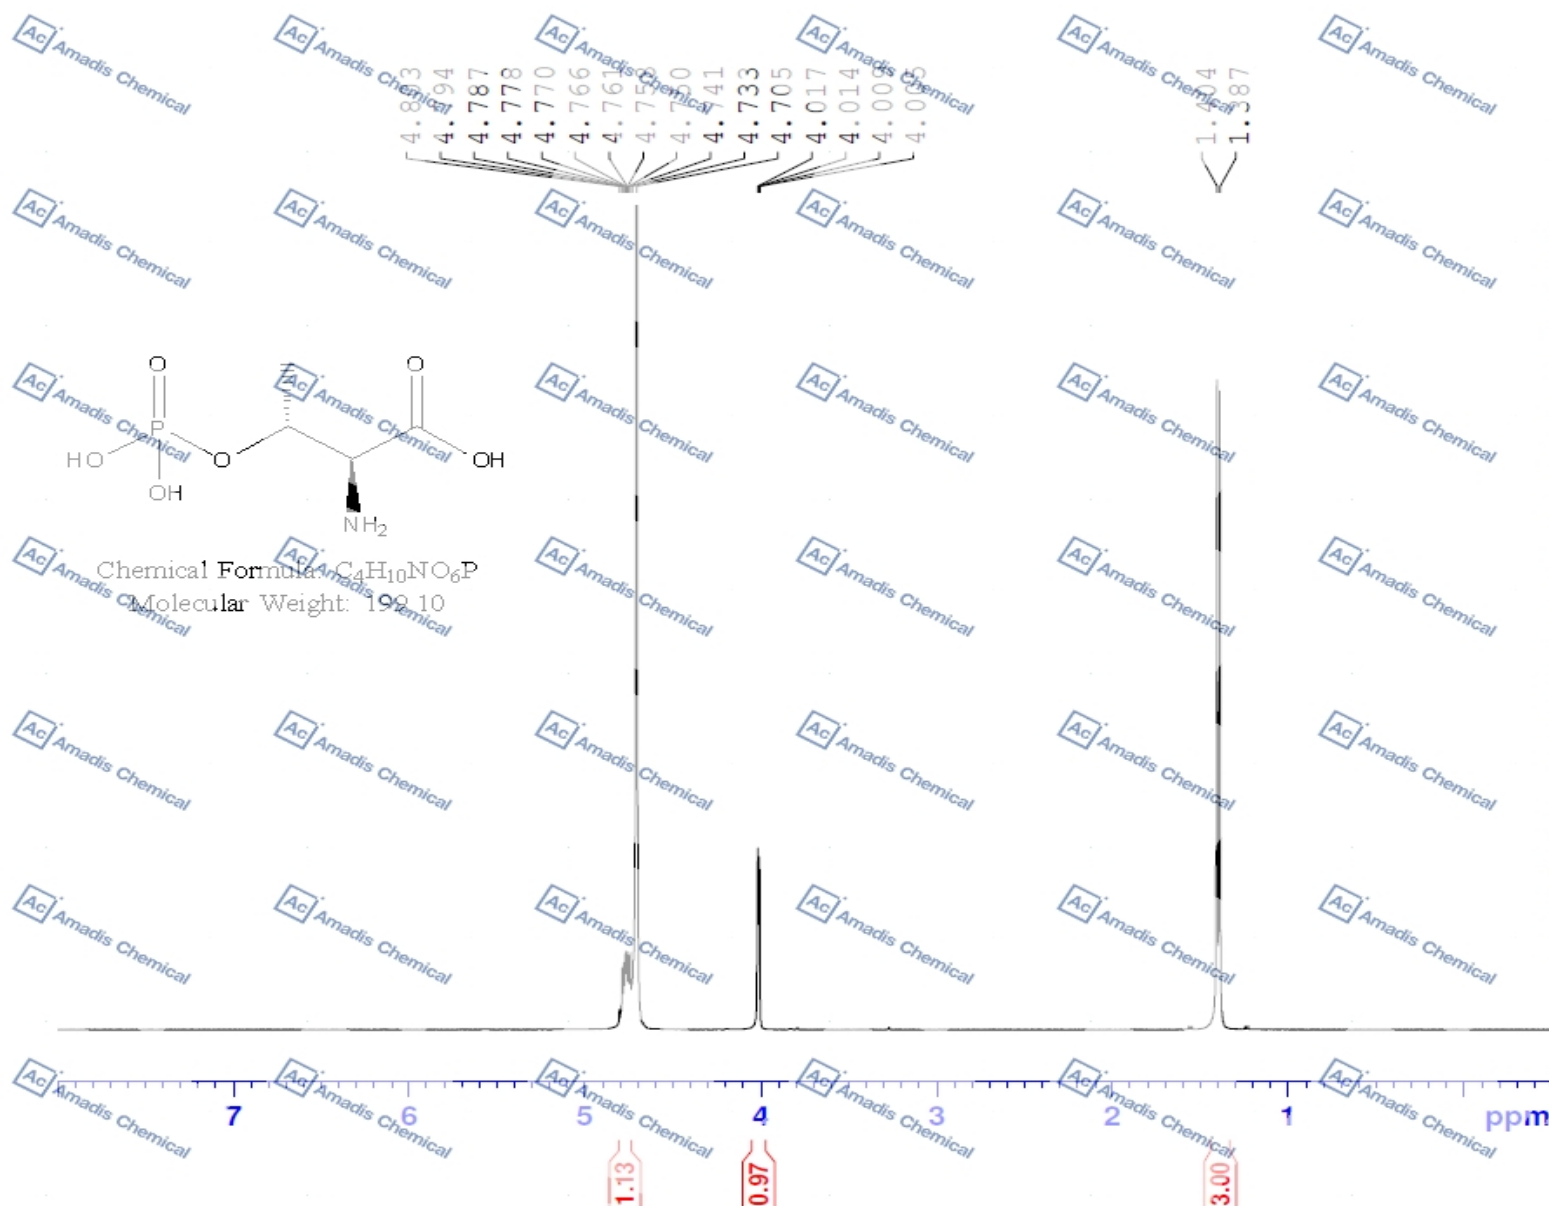

Current Data Parameters
NAME 0510-4745
EXPNO 20
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240511
Time 11.17 h
INSTRUM spect
PROBHD Z116098_0490
PULPROG zg30
TD 65536
SOLVENT D2O
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.2445 Hz
AQ 4.0894485 sec
RG 123.07
DW 62.400 usec
DE 6.50 usec
TE 299.7 K
D1 1.00000000 sec
TD0 1
SFO 400.1524703 MHz
NUC1 31P
P1 10.00 usec
PLW1 14.69799995 W

F2 - Processing parameters
SI 65536
SF 400.1500000 MHz
WDW EM
SS 0
LB 0.5 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.