




Current Data Parameters
 NAME 729610-40-6
 EXPNO 1400
 PROCNO 1
 F2 - Acquisition Parameters
 Date_ 20191206
 Time 10.22 h
 INSTRUM spect
 PROBHD zg30
 PULPROG zg30
 TD 32768
 SOLVENT CDCl3
 NS 3
 DS 0
 SWH 8012.820 Hz
 FIDRES 0.489064 Hz
 AQ 2.0447233 sec
 RG 130.5
 DW 62.400 usec
 DE 6.50 usec
 TE 292.6 K
 D1 2.00000000 sec
 TD0 1
 SF01 400.1330810 MHz
 NUC1 1H
 P1 3.33 usec
 PLW1 16.66200066 W
 F2 - Processing parameters
 SI 16384
 SF 400.1300000 MHz
 WDW EM
 SSB 0
 LB 0 Hz
 GB 0
 PC 1.00

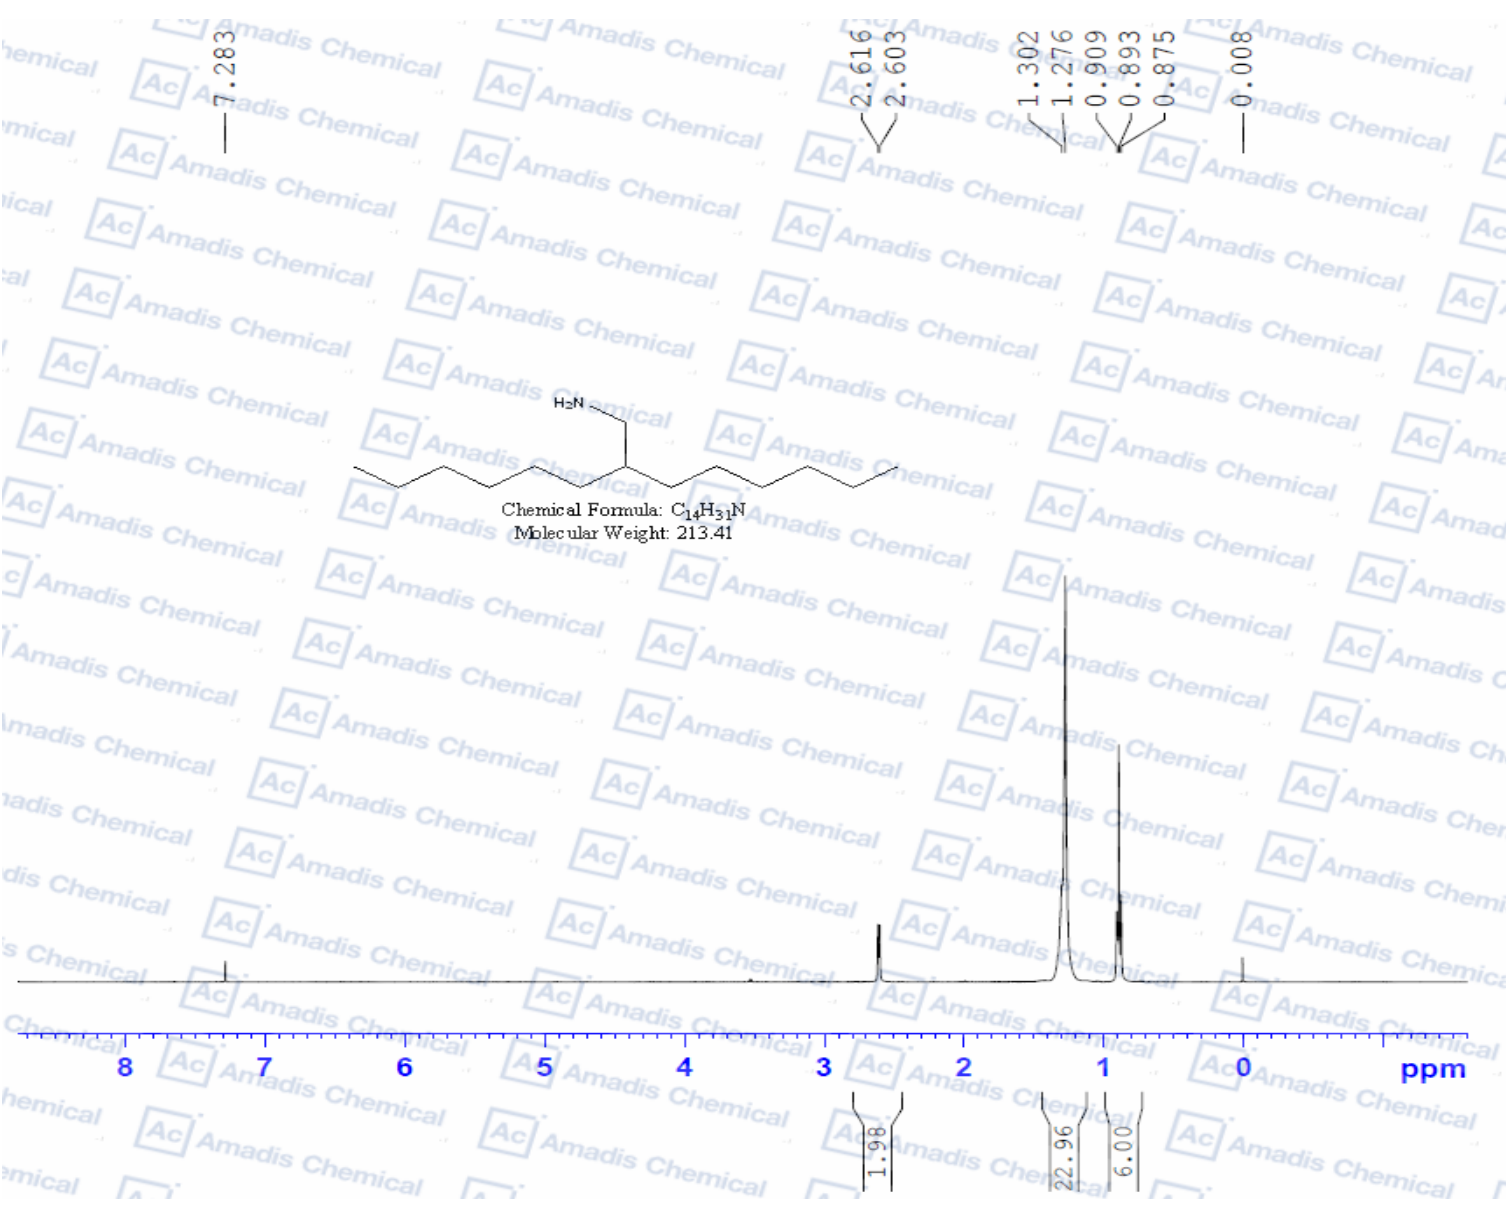

*For R&D use only