



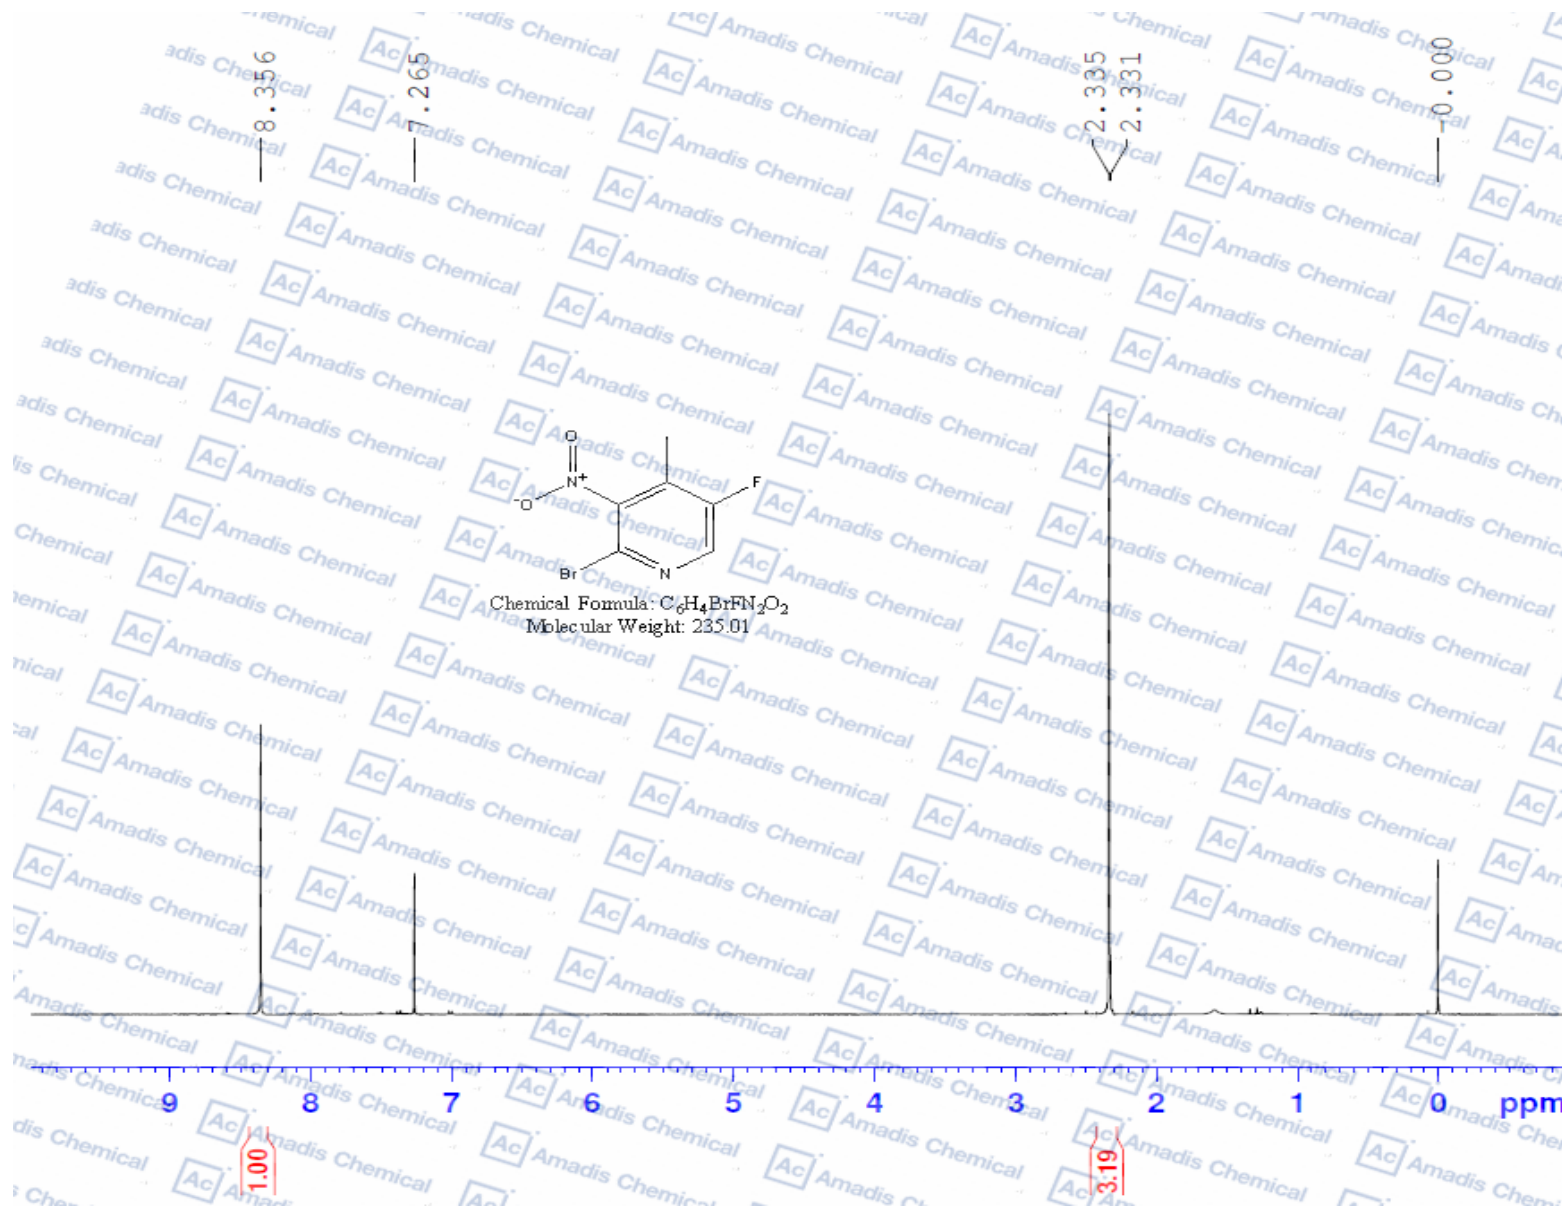

Current Data Parameters

EXPNO	1
PROCNO	1
F2 Acquisition Parameters	
Date_	20200805
Time	11.01
INSTRUM	spect
PROBHD	5 mm PABBO BB/
PULPROG	zg30
TD	65536
SOLVENT	CDCl3
NS	16
DS	2
SWH	8012.820 Hz
FIDRES	0.122266 Hz
AQ	4.0894465 sec
RG	116.94
DW	62.400 usec
DE	6.50 usec
TE	295.4 K
D1	1.00000000 sec
TD0	1
===== CHANNEL f1 =====	
SFO1	400.1324710 MHz
NUC1	1H
PI	10.00 usec
PLW1	16.00000000 W
F2 Processing parameters	
SI	65536
SF	400.1300078 MHz
WDW	EM
SSB	0
LB	0.30 Hz
GB	0
PC	1.00

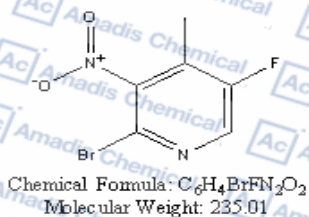

\*For R&D use only