



Current Data Parameters

```



EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210708
Time 12.54
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 102.33
DW 62.400 usec
DE 6.50 usec
TE 293.9 K
D1 1.00000000 sec
TDO 1

===== CHANNEL f1 =====
SFO1 400.1324710 MHz
NUC1 1H
P1 10.00 usec
PLW1 16.00000000 W

F2 - Processing parameters
SI 65536
SF 400.1300018 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00
    
```

12.302
6.584
4.871
3.570
3.544
3.499
3.472
3.343
2.512
2.508
2.503
2.499
2.494
1.365
1.286
0.000

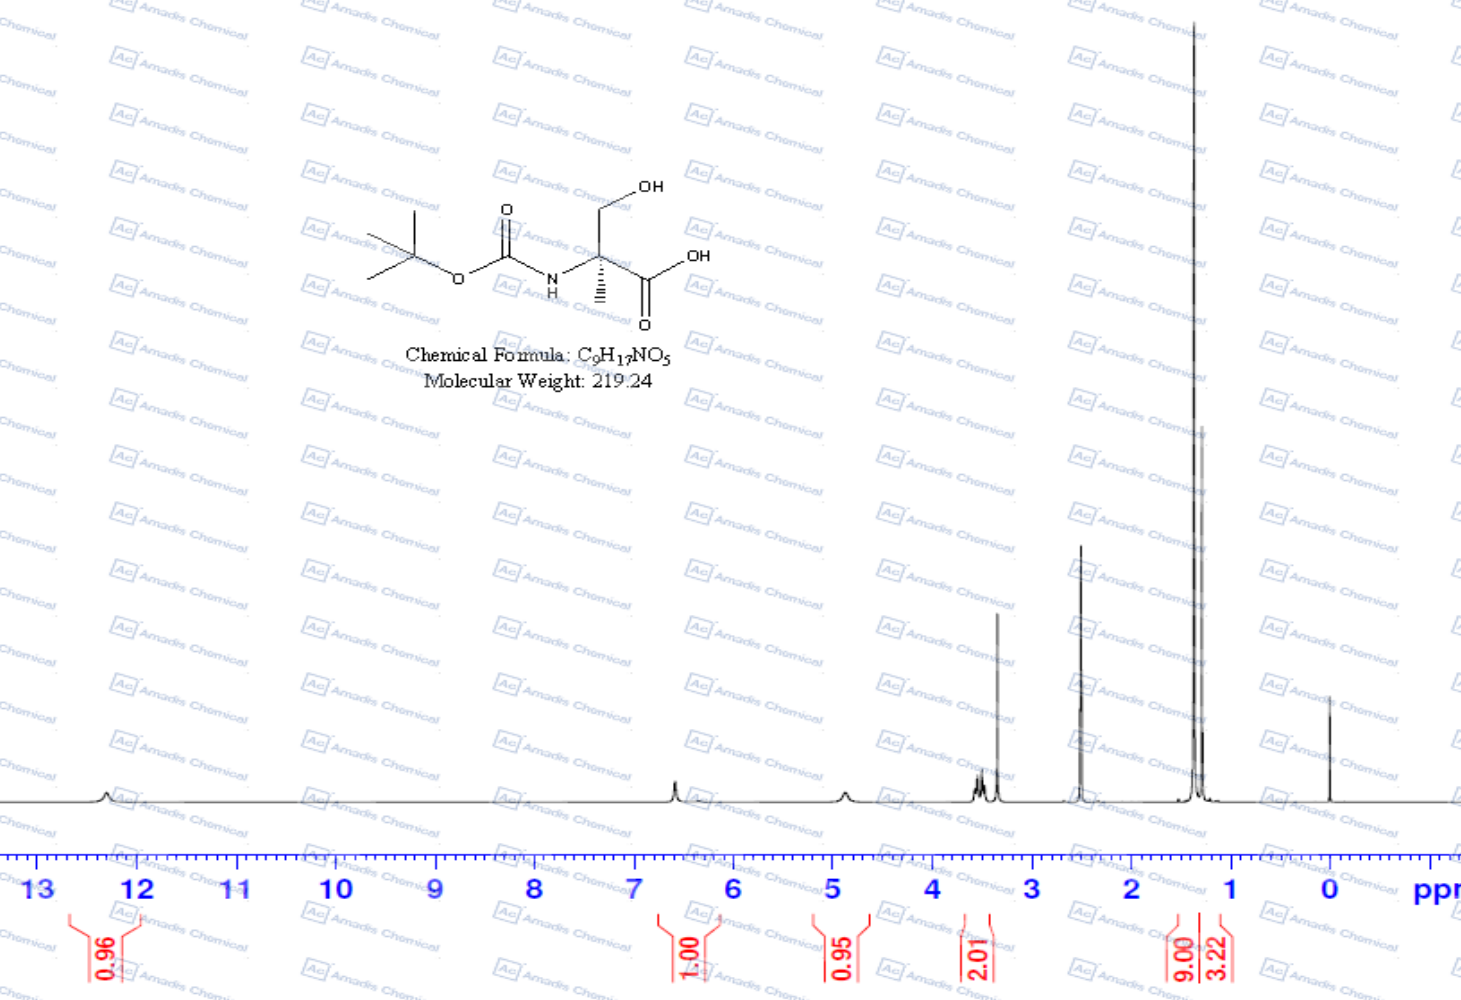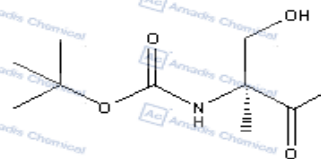

*For laboratory or manufacturing use only, not for drug, food and household use.