
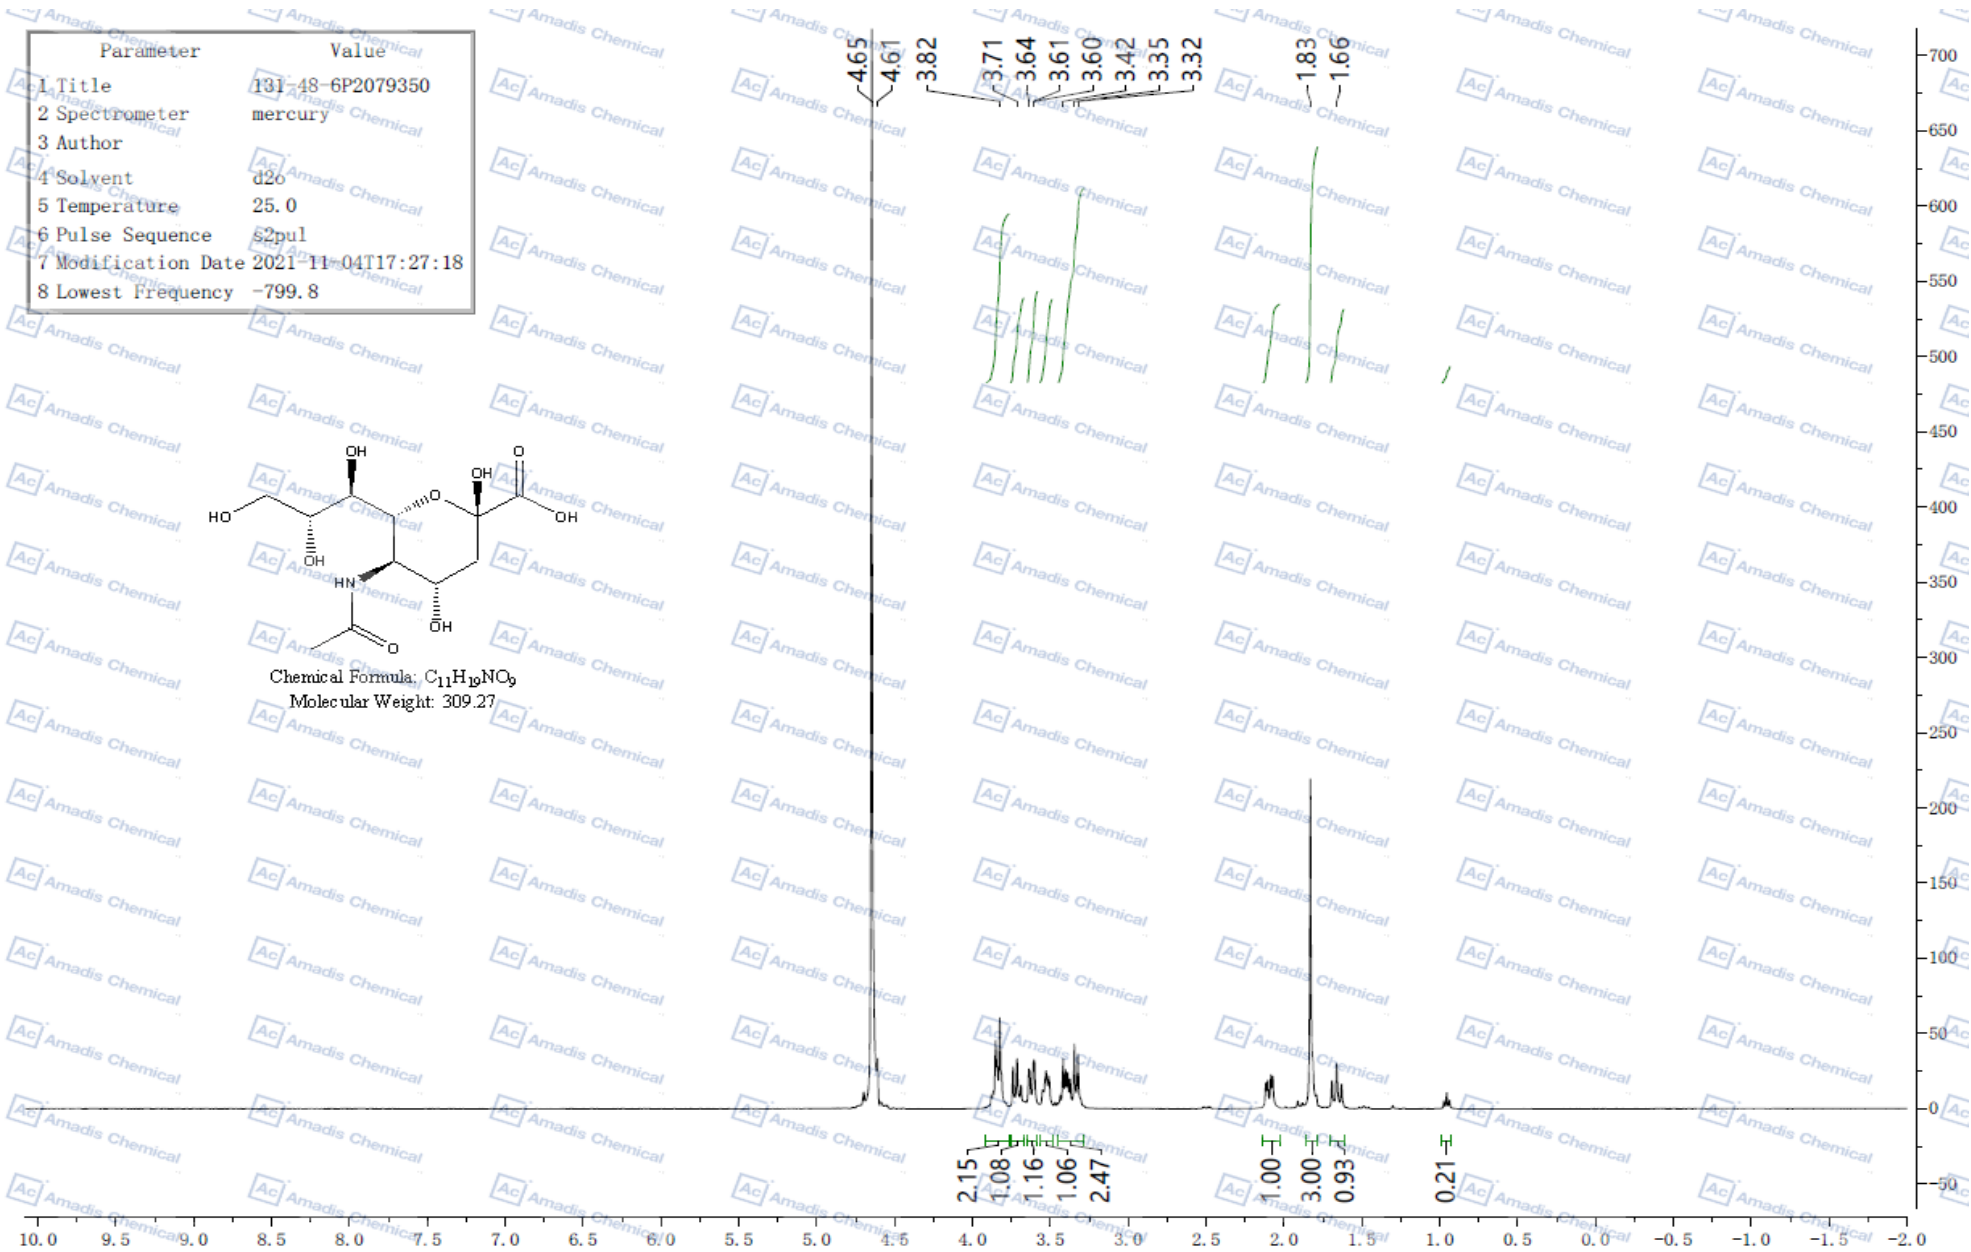


Parameter	Value
1 Title	131-48-6P2079350
2 Spectrometer	mercury
3 Author	
4 Solvent	d2o
5 Temperature	25.0
6 Pulse Sequence	s2pul
7 Modification Date	2021-11-04T17:27:18
8 Lowest Frequency	-799.8

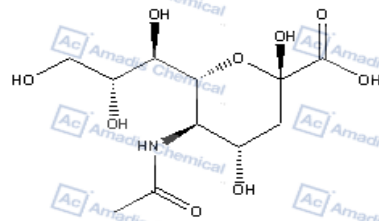

\*For laboratory or manufacturing use only, not for drug, food and household use.