



Current Data Parameters


```

EXPNO          3
PROCNO         1

F2 - Acquisition Parameters
Date_          20221017
Time           11.00
INSTRUM        spect
PROBHD         5 mm PABBO BB/
PULPROG        zg30
ID             65536
SOLVENT        CDCl3
NS             16
DS             2
SWH            8012.820 Hz
FIDRES         0.122266 Hz
AQ             4.0894465 sec
RG             91.2
DW             62.400 usec
DE             6.50 usec
TE             294.2 K
D1             1.00000000 sec
TD0            1

===== CHANNEL f1 =====
SFO1           400.1324710 MHz
NUC1            1H
P1             10.00 usec
PLW1           16.00000000 W

F2 - Processing parameters
SI             65536
SF             400.1300104 MHz
WDW            EM
SSB            0
LB             0.30 Hz
GB             0
PC             1.00
    
```

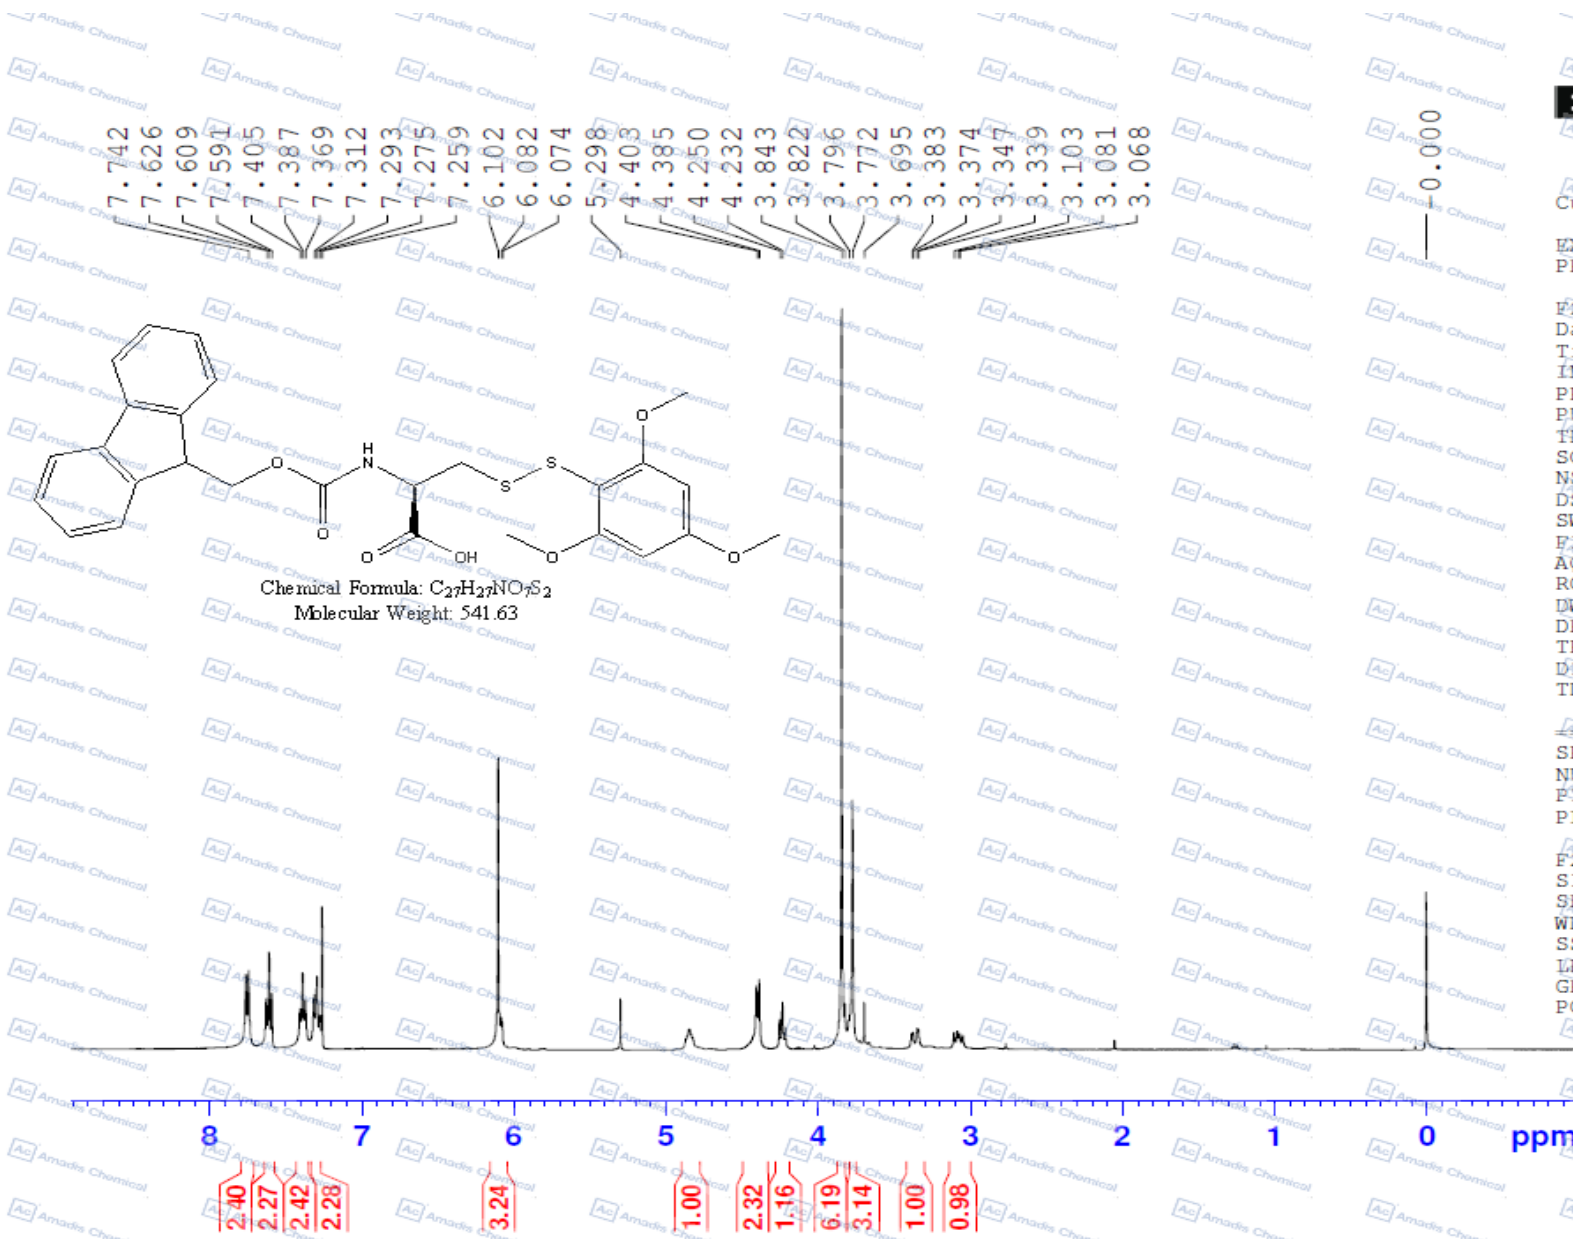

*For laboratory or manufacturing use only, not for drug, food and household use.