




Current Data Parameters  
NAME 0306-4  
EXPNO 10  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20240307  
Time 14.26 h  
INSTRUM spect  
PROBHD E116098\_042001  
PULPROG zgpg30  
TD 65536  
SOLVENT CDCl3  
NS 16  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 4.089465 sec  
RG 128  
DW 62.400 sec  
DE 6.50 usec  
TE 295.3 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1524709 MHz  
NUC1 1H  
PC 14.69799565 W

F2 - Processing parameters  
SI 65536  
SF 400.1500077 MHz  
WDW EM  
SSB 0  
LF 0.30 Hz  
GB 0  
PC 1.00

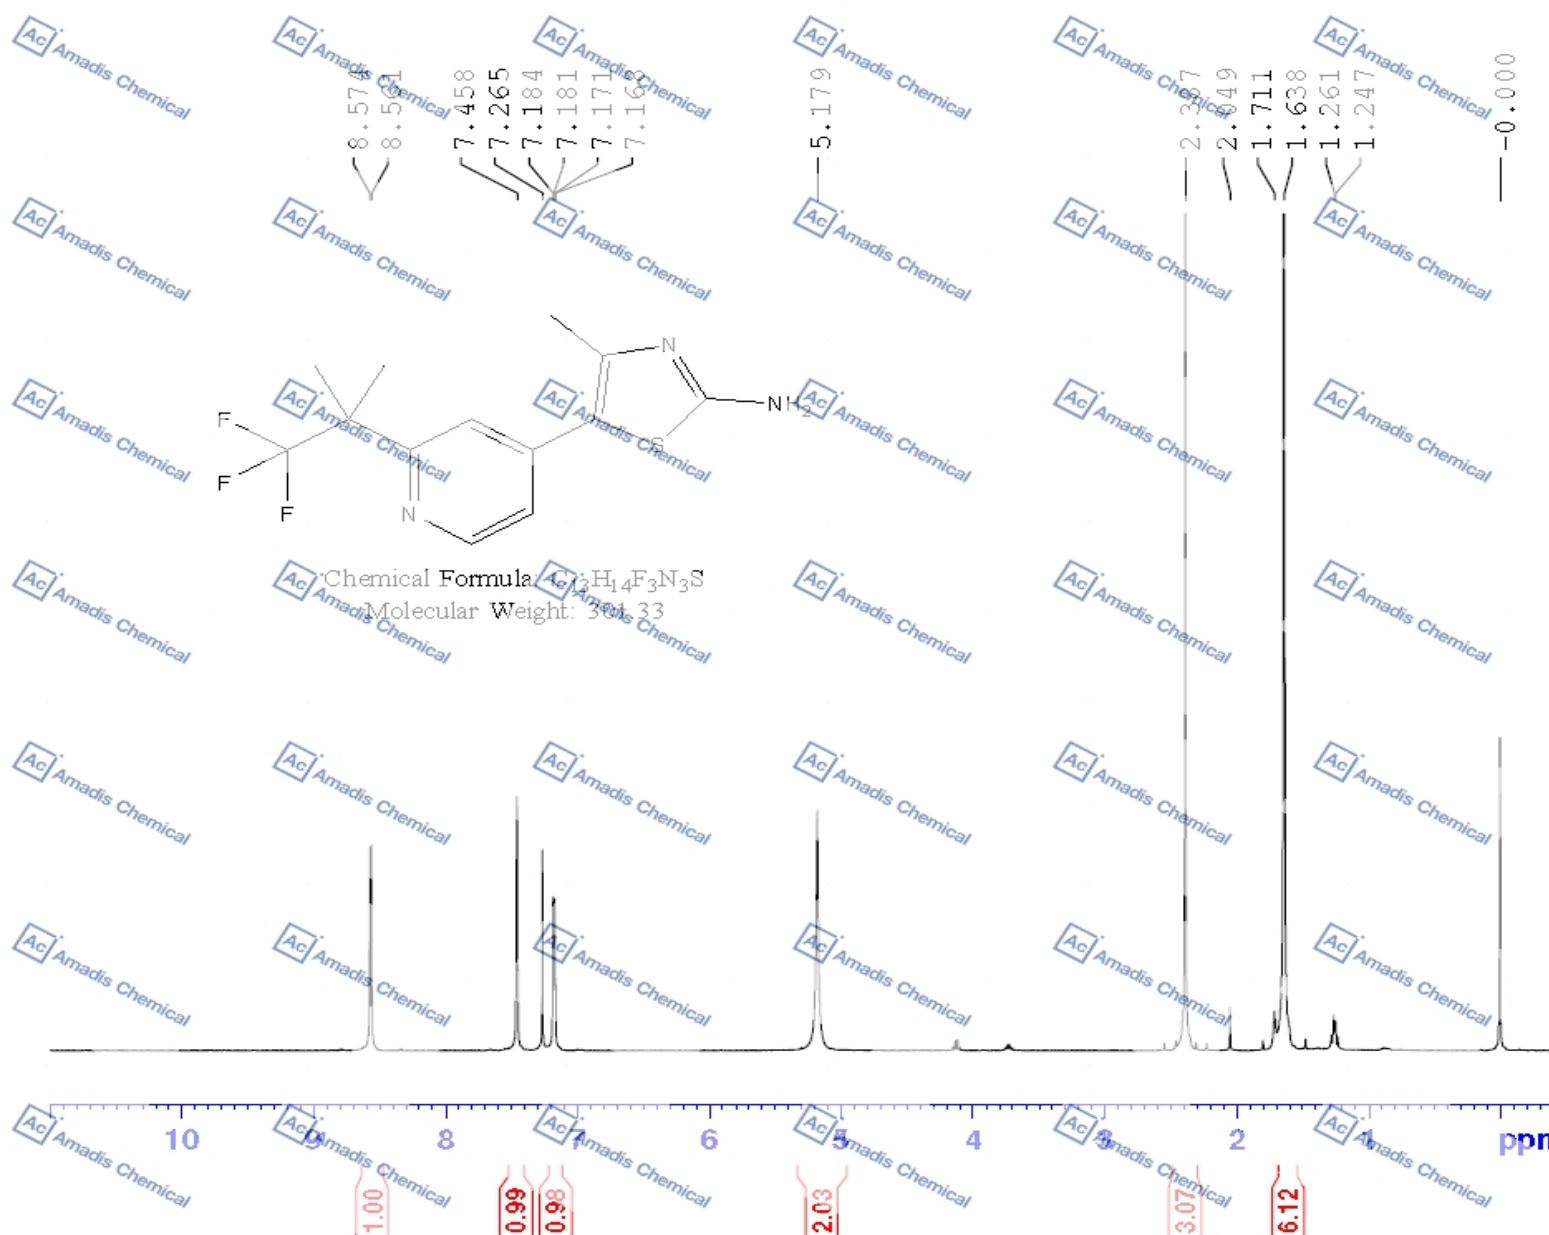

\*For laboratory or manufacturing use only, not for drug, food and household use.