


MS of 1001600-56-1

MASS SPECTROMETRY REPORT

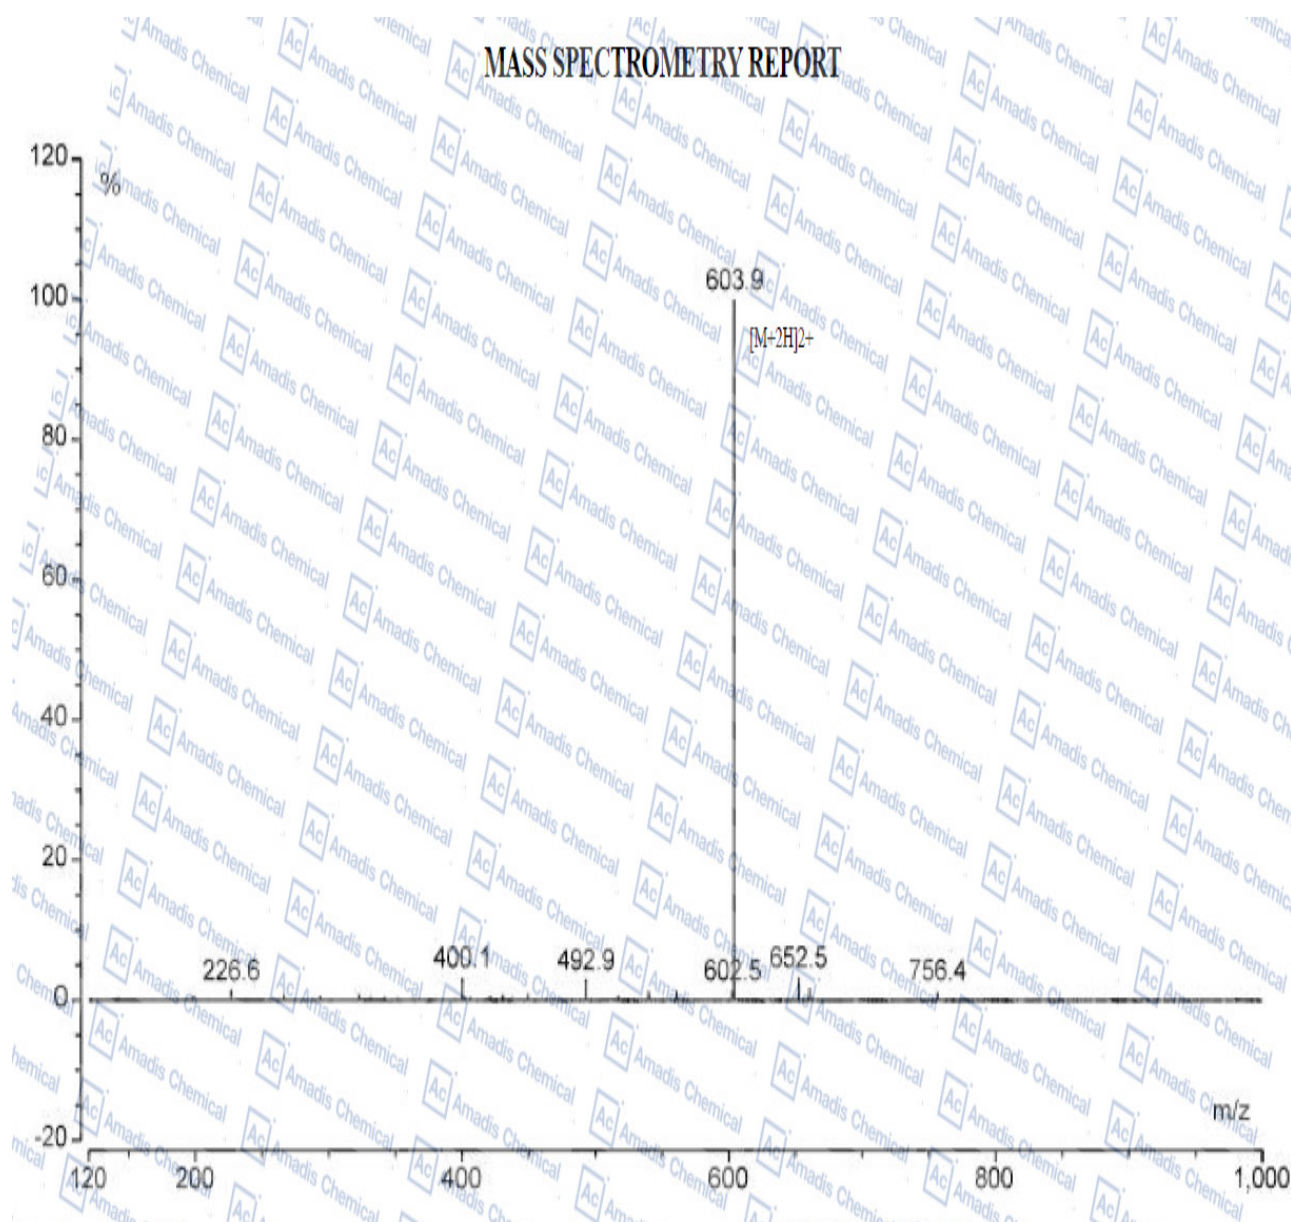

Sample Description

Analyzed date: 2020-8-4

Analyst: SHAO

Sample: 602649

M.W.: 1205.6

Lot No.:

Instrument SHIMADZU LCMS-2020

Probe: ESI

Nebulizer Gas Flow: 1.5L/min

CDL: -20.0v

CDL Temp.: 250°C

Block Temp.: 200°C

Probe Bias: +4.5kv

Detector: 1.5kv

T. Flow: 0.2ml/min

B. Conc.: 50%H₂O/50%ACN

*For R&D use only

*if you have any comments and suggestions, please contact us by sales@amadischem.com