


MS of 2089648-75-7

Name: 11 Rack Pos.: Instrument: Instrument 1 Operator: Instrument 1
Inj. Vol. (ul): 1 Plate Pos.: IRM Status: All ions missed
Data File: 20210817b-002.d Method (Acq): positive quick run for hplc purified sample with ref MASS 2min.m Comment: Acq. Time (Local): 8/18/2021 2:44:03 PM (UTC+08:00)

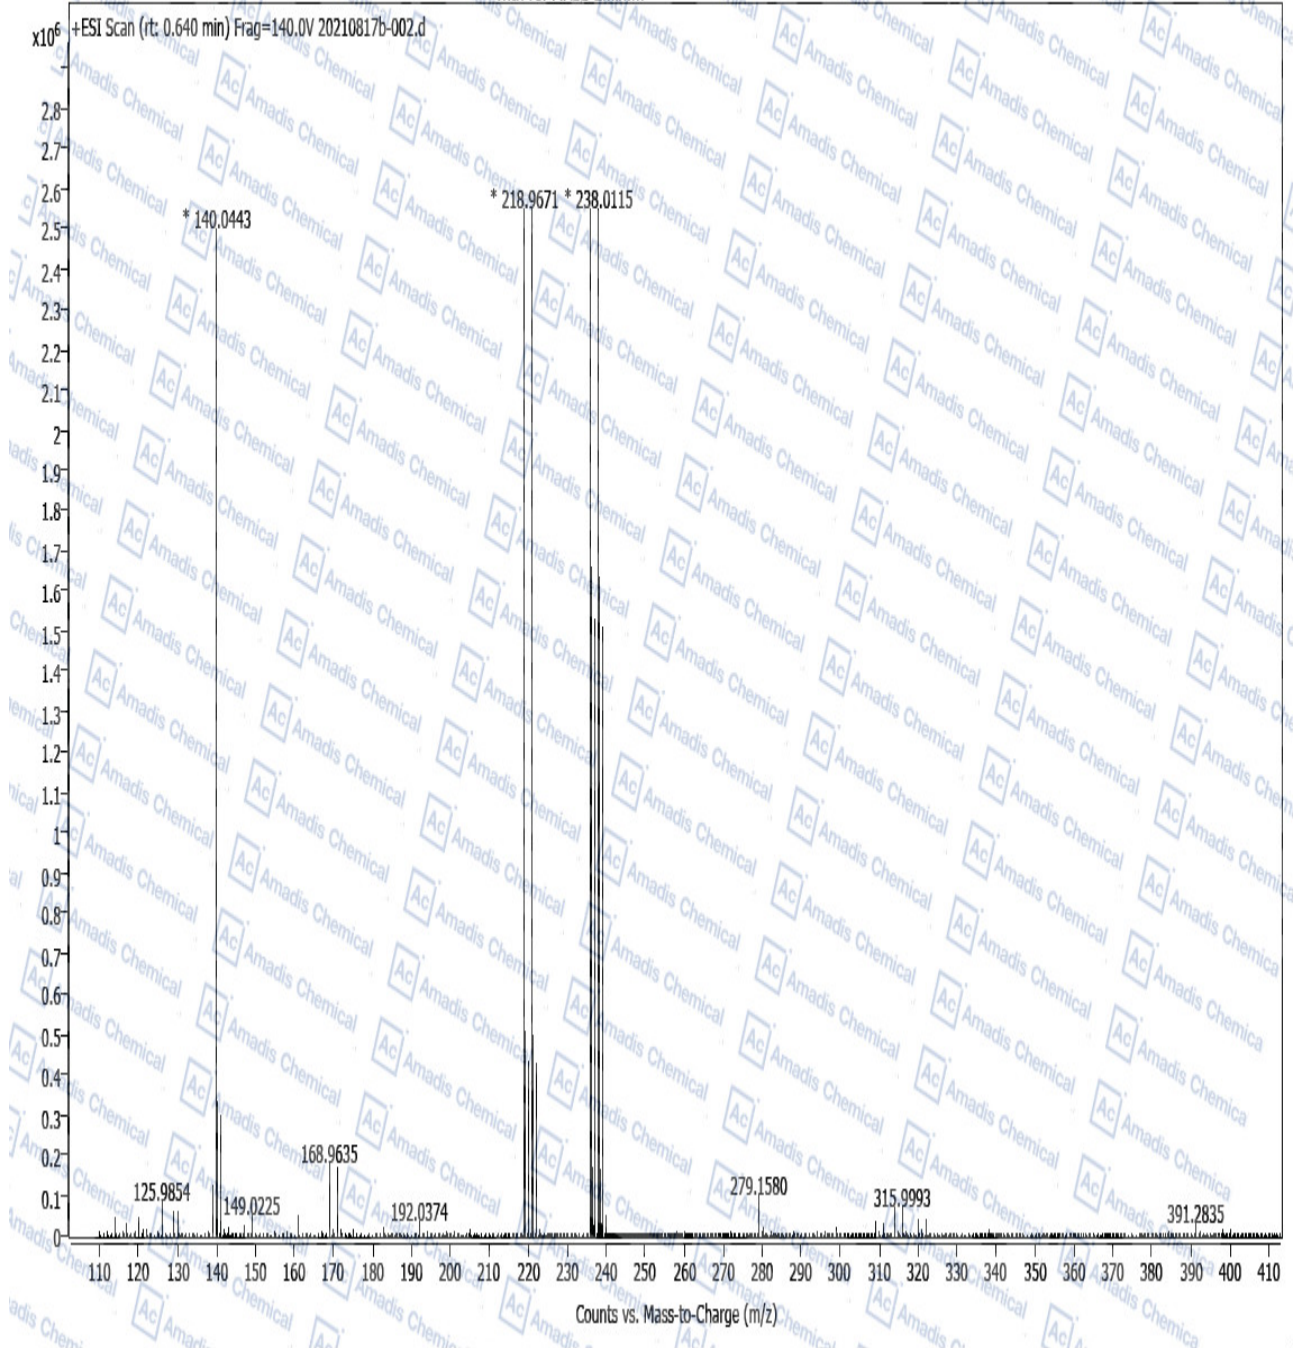

*For R&D use only

*if you have any comments and suggestions, please contact us by sales@amadischem.com