




LCMS of 957-77-7

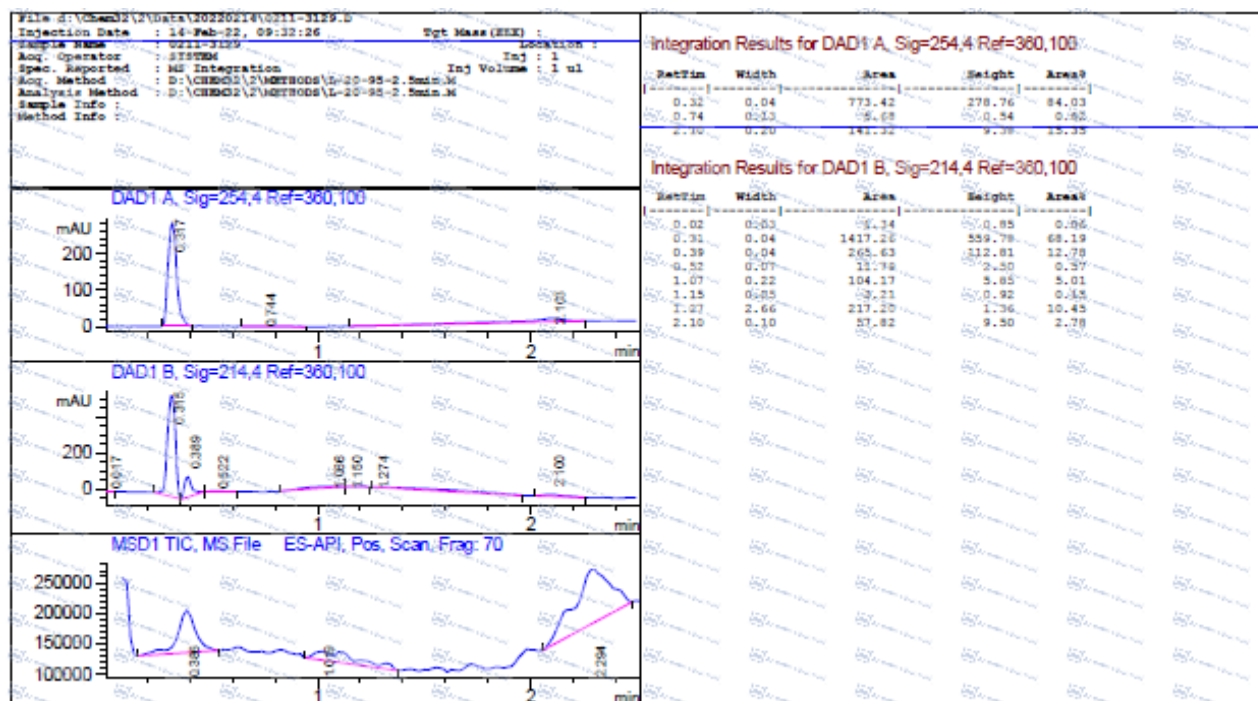


Ret. Time: 0.39 <<<< POSITIVE SPECTRA >>>>

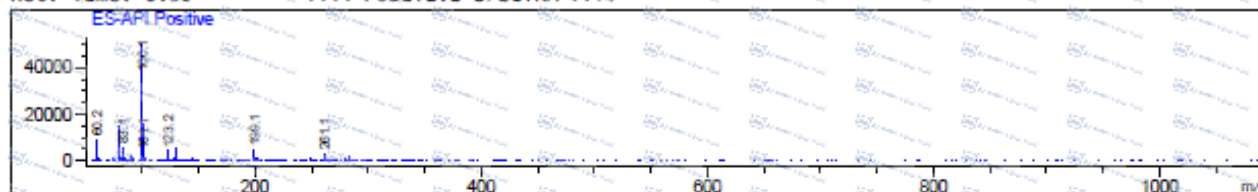

Ret. Time: 1.02

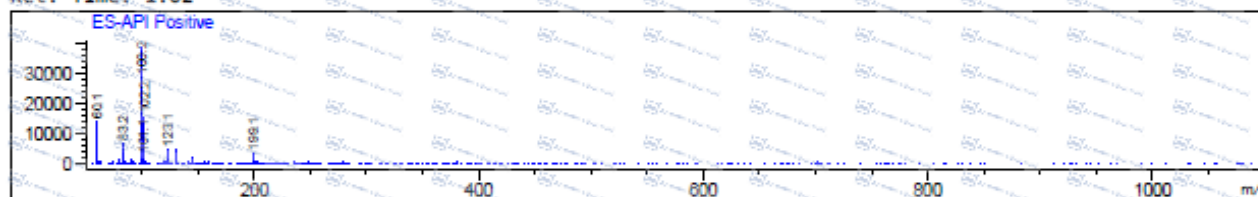

Ret. Time: 2.29

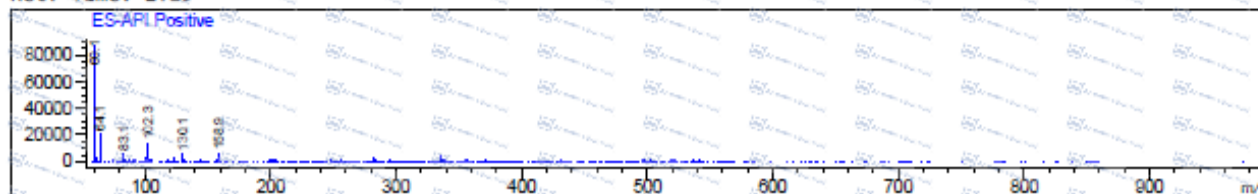

*For laboratory or manufacturing use only, not for drug, food and household use.

*if you have any comments and suggestions, please contact us by sales@amadischem.com