


MS OF 83150-76-9

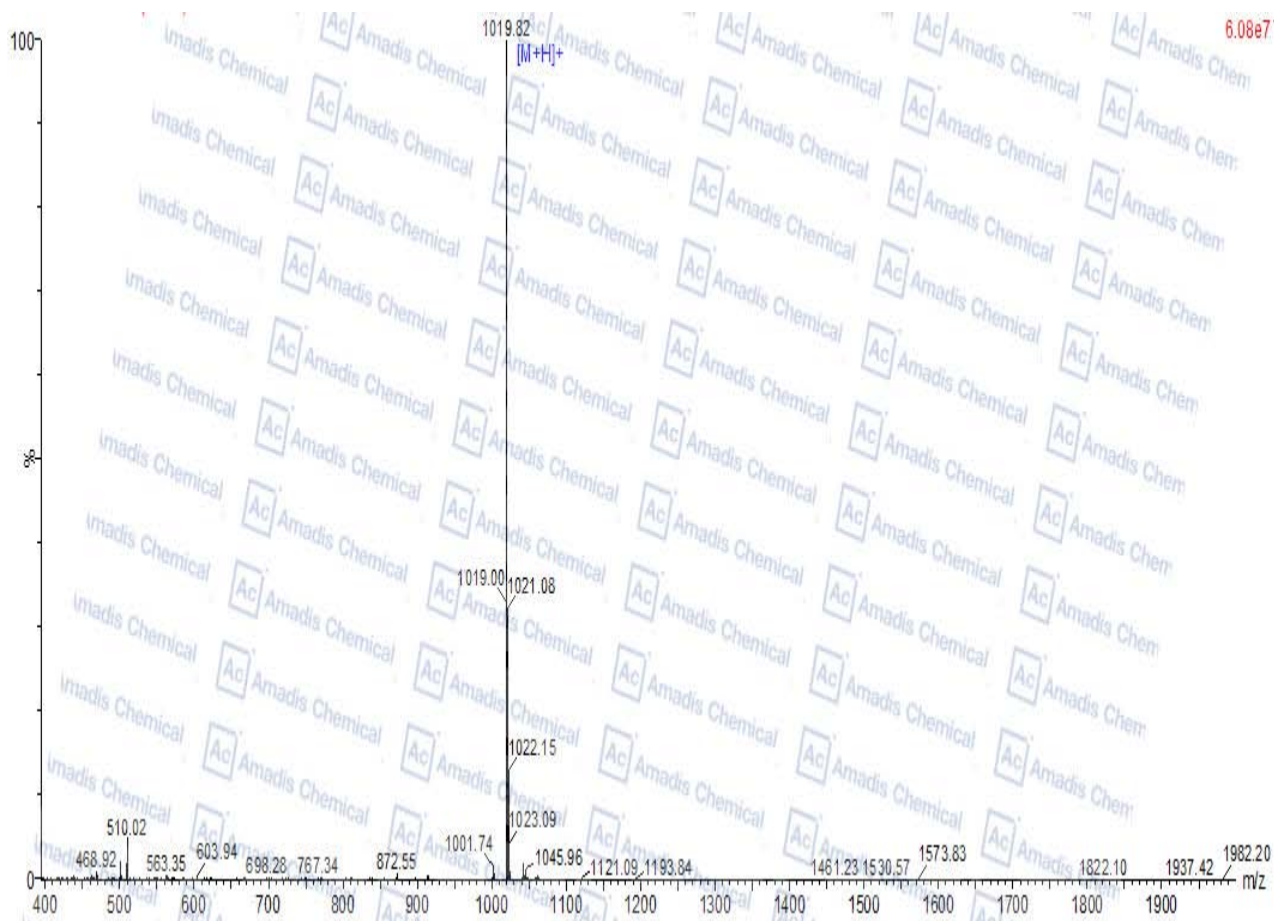

Sample Description:	Instrument:	Waters ZQ2000	
Analyzed date:	Probe:	ESI	Probe Bias: +4.5kv
Analyst:	Nebulizer Gas Flow:	1.5L/min	Detector: 1.5kv
Sample:	CDL:	-20.0v	T. Flow: 0.2ml/min
M.W.:	CDL Temp.:	250.0C	B. Conc.: 50%H2O/50%ACN
Lot No.:	Block Temp.:	200.0C	

* If you have any comments and suggestions, please contact us by sales@amadischem.com