


MS of 195868-13-4

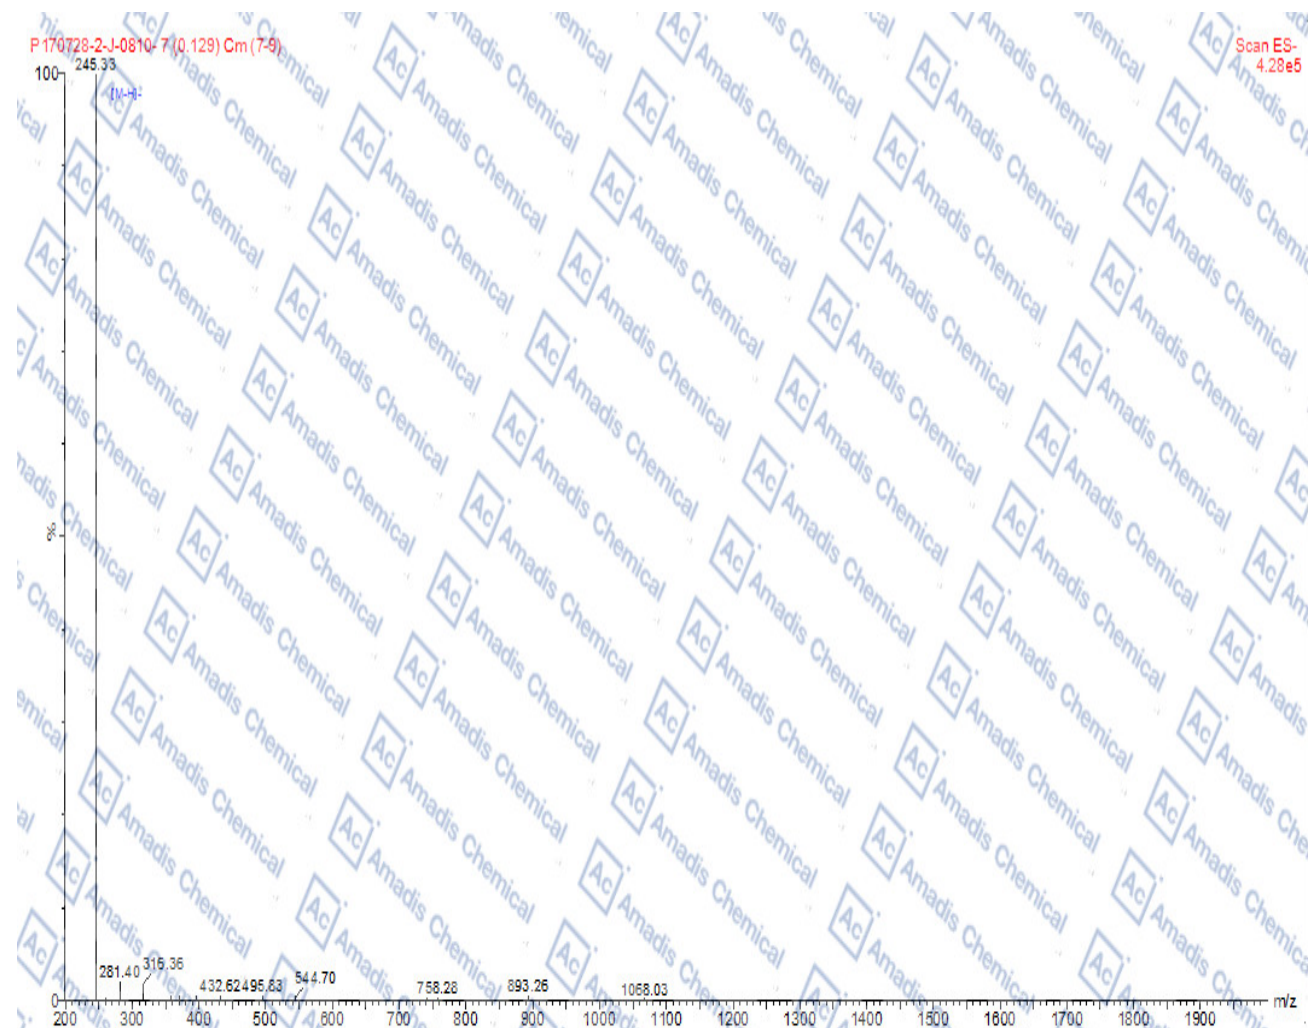

Sample Description:	Instrument:	Waters ZQ2000	
Analyzed date:	Probe:	ESI	Probe Bias: +4.5kv
Analyst:	Nebulizer Gas Flow:	1.5L/min	Detector: 1.5kv
Sample:	CDL:	-20.0v	T. Flow: 0.2ml/min
M.W.:	CDL Temp.:	250°C	B. Conc.: 50%H ₂ O/50%ACN
Lot. No.:	Block Temp.:	200°C	

* If you have any comments and suggestions, please contact us by sales@amadischem.com