


HPLC of 22987-10-6

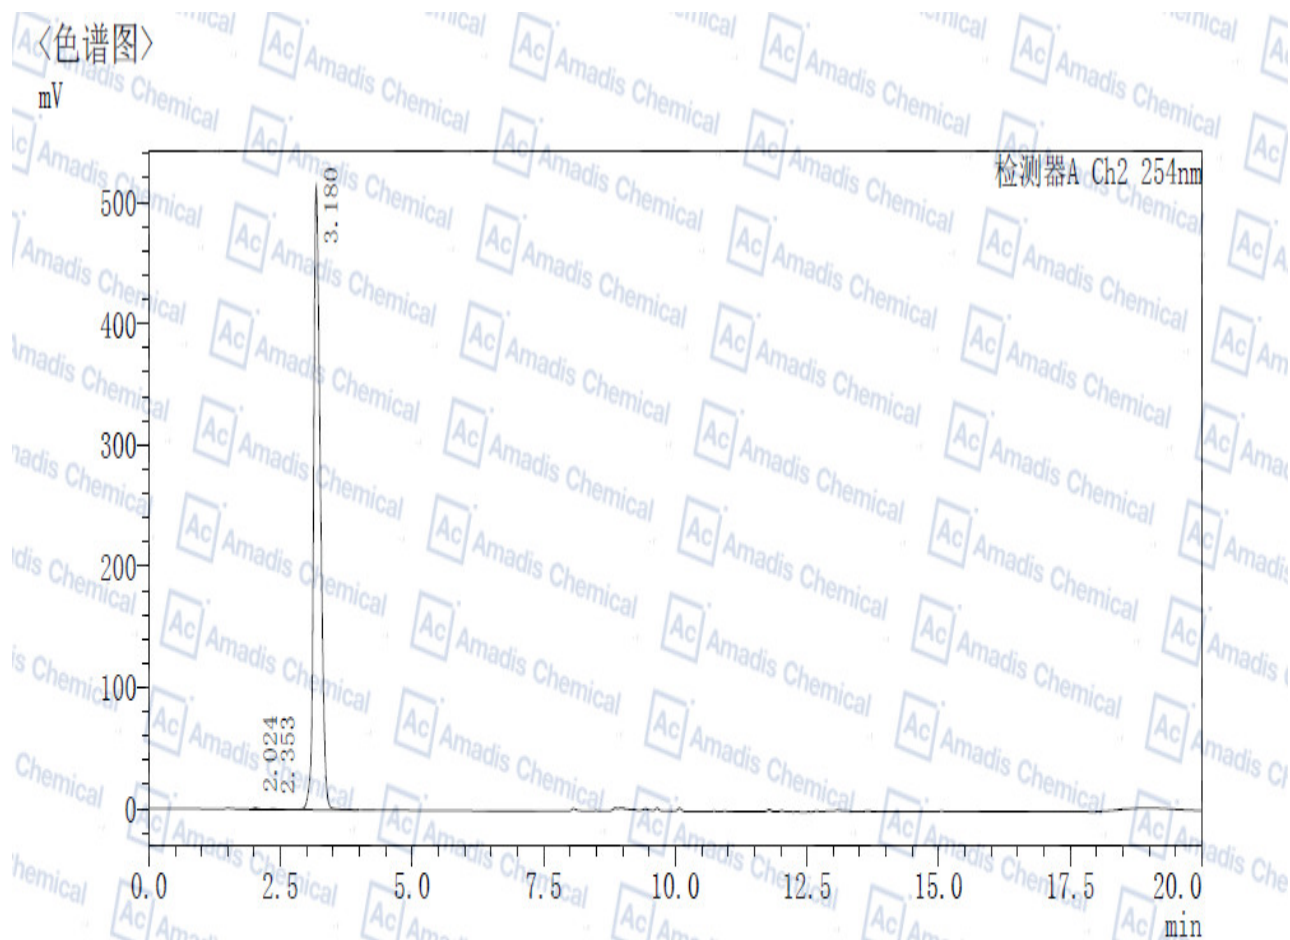

〈峰表〉

检测器A Ch2-254nm

峰号	保留时间	面积	高度	浓度	面积%
1	2.024	5639	1106	0.122	0.122
2	2.353	1447	202	0.031	0.031
3	3.180	4614888	514409	99.847	99.847
总计		4621974	515717		100.000

*For R&D use only

*if you have any comments and suggestions, please contact us by sales@amadischem.com