


HPLC of 53123-88-9

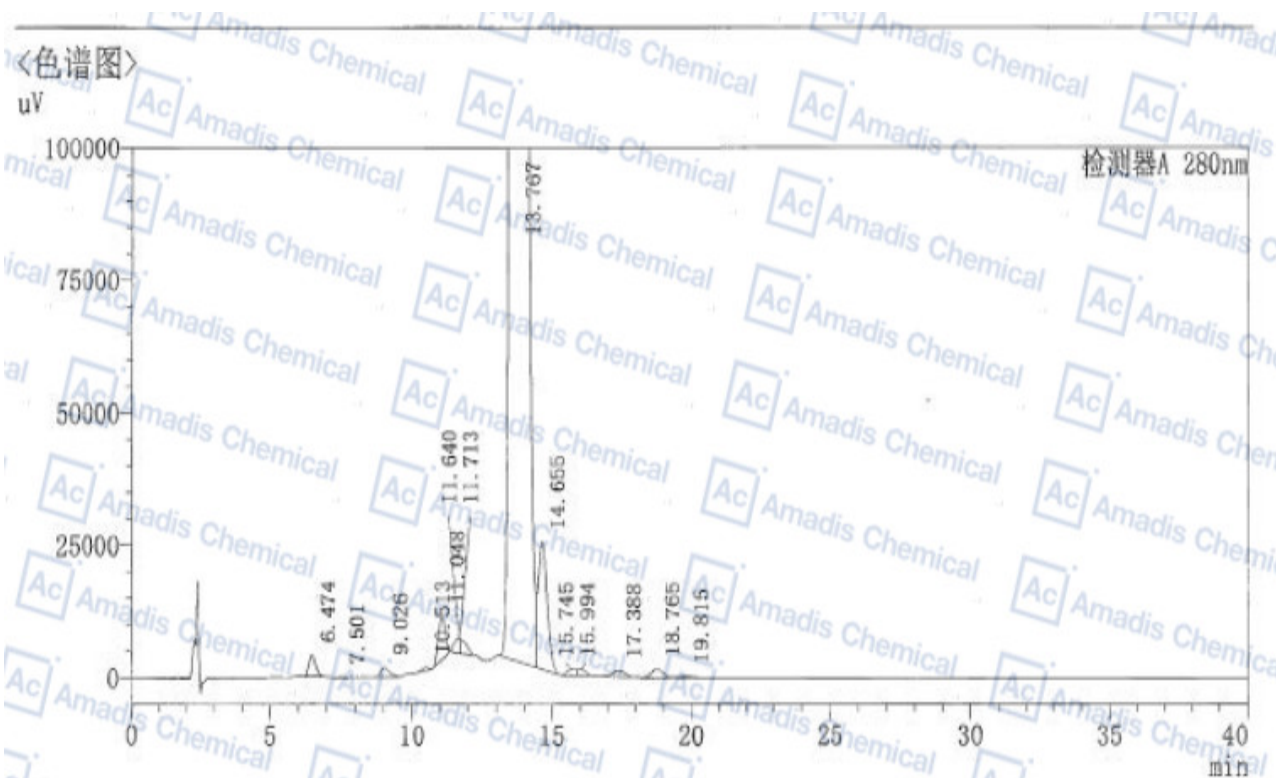

<峰表>

检测器A 280nm

峰号	保留时间	理论塔板数(USP)	分离度(USP)	面积	面积%	化合物名
1	6.474	3465	—	62142	0.210	
2	7.501	5956	2.478	1556	0.034	
3	9.026	4826	3.356	37400	0.127	
4	10.513	9341	3.116	8466	0.068	
5	11.048	9587	1.207	133107	0.346	林+品+大+单
6	11.640	115	0.247	37307	0.126	
7	11.713	—	—	38687	0.131	
8	13.767	6843	—	28515409	96.934	Jx59
9	14.655	6624	1.281	555204	1.662	C+品+单
10	15.745	75	0.273	24985	0.085	
11	15.994	1390	0.056	24369	0.083	
12	17.388	6561	1.083	32607	0.162	
13	18.765	9028	1.671	46708	0.158	
14	19.815	6591	1.189	13121	0.044	
总计				29531068	100.000	

*For R&D use only

*If you have any comments and suggestions, please contact us by sales@amadischem.com