


HPLC of 1659305-78-8

Data file: E:\DATA\200224\602607_20010002Final.D
Sample name: 602607_20010002Final
Description: Mobile phase: Buffer A: 0.1%TFA in H2O
 Buffer B: 0.1%TFA in ACN
 Gradient: 29-39% B in 20min, Flow rate: 1.0ml/min
 Column: Unitary C18, 4.6*150mm, 5um 100A (A-006)
 Instrument: Agilent HPLC 1100
Instrument: QC **Location:** 81
Injection date: 2020/2/24 16:03:39 **Injection:** 1 of 1
Last changed: 2020/2/24 17:07:18 **Injection volume:** 10.000
Acq. operator: QC_1

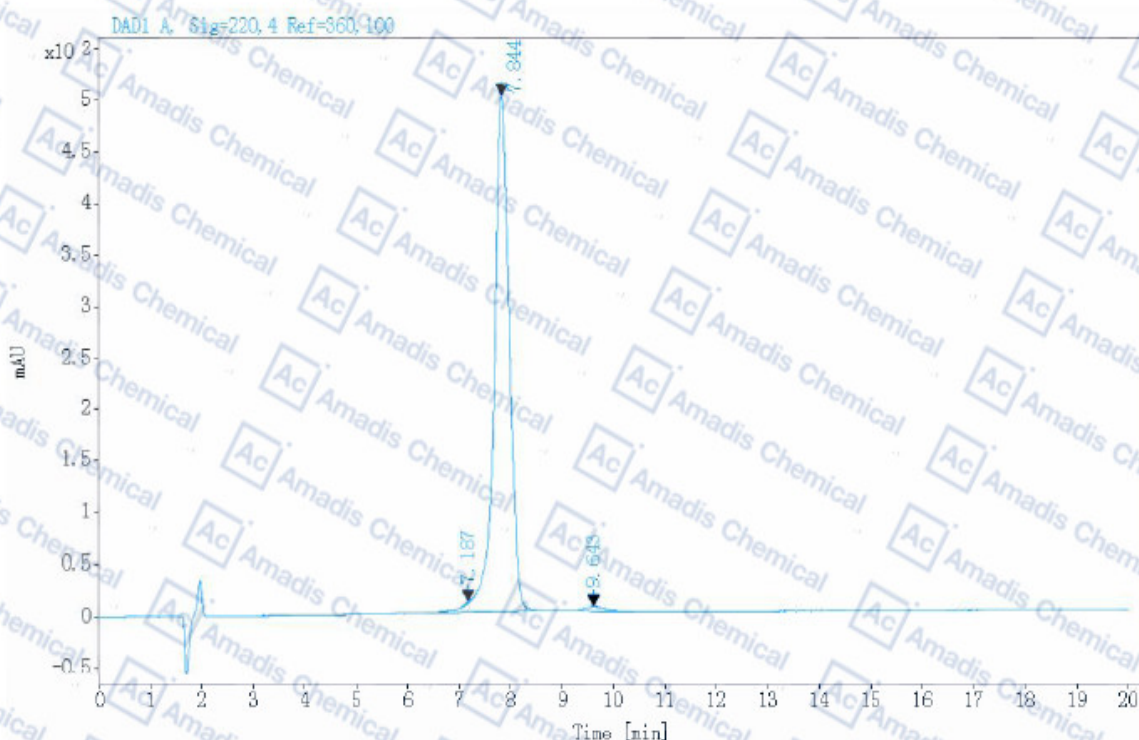

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area%	Name
1.187	VV E	0.1330	18.7454	1.8689	0.1798	
7.844	VB R	0.3138	10268.0674	495.5196	98.4951	
9.643	VB R	0.4291	138.1444	4.8390	1.3251	
Sum			10424.9572			

*For R&D use only

*If you have any comments and suggestions, please contact us by sales@amadischem.com