


### HPLC of 1001600-56-1

**Data file:** C:\CHEMS2\1\DATA\200804\602649\_20070051Final.D  
**Sample name:** 602649\_20070051Final  
**Description:** Mobile phase: Buffer A: 0.1%TFA in H2O, Buffer B: 0.1%TFA in ACN  
 Gradient: 40-50% B in 20min, Flow rate: 1.0ml/min  
 Column: Unitary C18, 4.6\*150mm, 5um 100A (A-007)  
 Instrument: Agilent HPLC 1100  
**Instrument:** 1100 **Location:** C11  
**Injection date:** 2020/8/4 8:54:34 **Injection:** 1 of 1  
**Last changed:** 2020/8/4 9:24:43 **Injection volume:** 10.000  
**Acq. operator:** qc

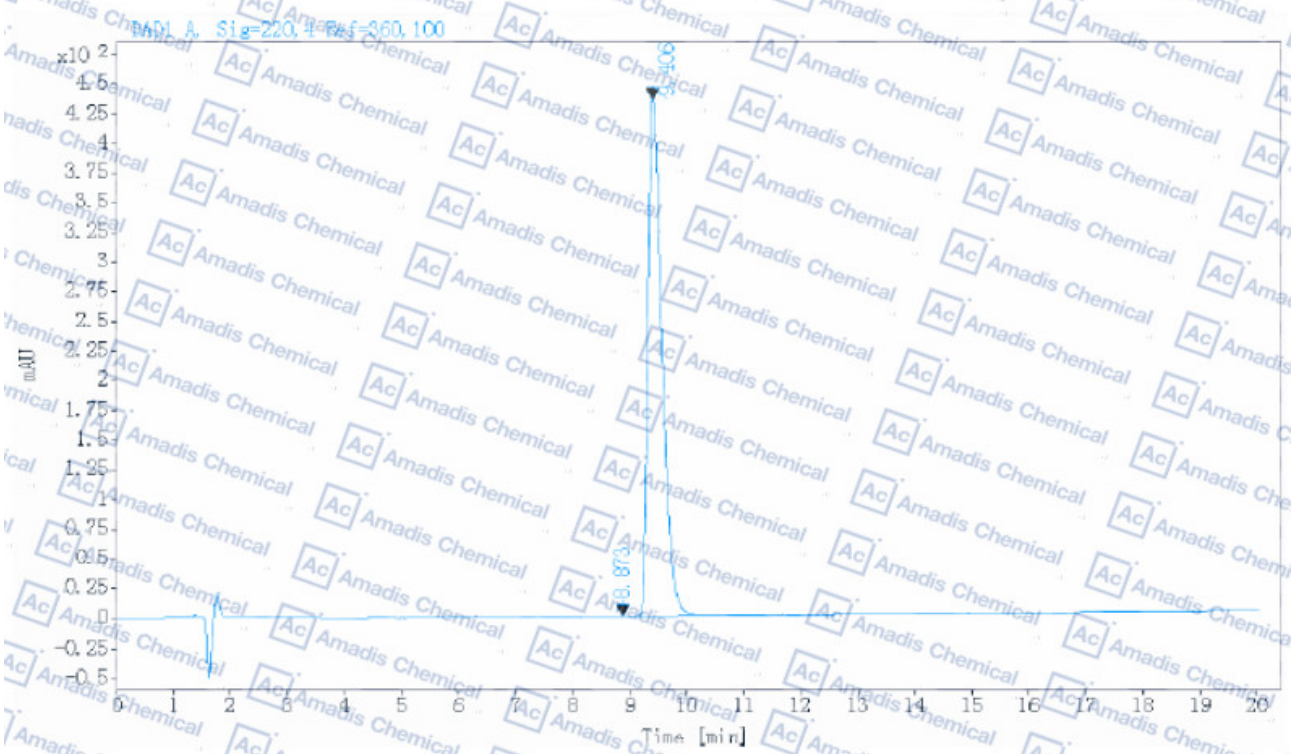

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area%	Name
8.873	MF	0.1906	4.4486	0.3889	0.0593	
9.106	FM	0.2795	7496.8296	446.9627	99.9407	
Sum			7501.2782			

\*For R&D use only

\*if you have any comments and suggestions, please contact us by [sales@amadischem.com](mailto:sales@amadischem.com)