


HPLC of 1193447-34-5

GLXC-02033 HPLC Report

Column: Zorbax Eclipse XDB-CN, 5µm, 4.6 x 250 mm

Phase A: Chloroform ; Phase B: Hexanes , A:B= 45:55 (v/v)

Flow Rate: 1 mL/min; Detector Ch1: 254 nm

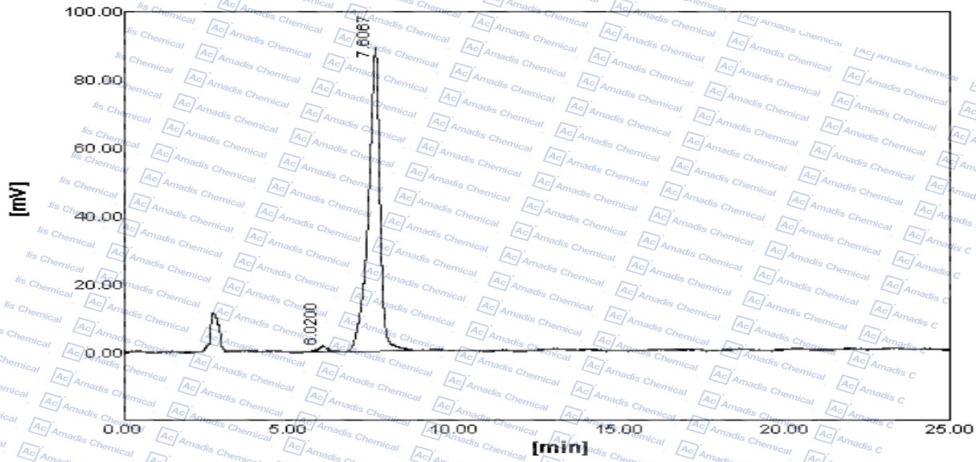

Sample Concentration: 250µg in 1 mL chloroform

	RT (min)	AREA (mV x sec)	AREA (%)	Thereo. Plates	Tailing Factor
1	6.0200	35.5919	1.60	2030.9	1.2376
2	7.6067	2187.7266	98.40	3146.0	0.7881
SUM		2223.3184			

*For R&D use only

* if you have any comments and suggestions, please contact us by sales@amadischem.com