


HPLC of 1639939-40-4

Data file: D:\CHEM32\1\DATA\220517\605024_22040024Final.D
 Sample name: 605024_22040024Final
 Description: Mobile phase: Buffer A: 0.1%TFA in H2O
 Buffer B: 0.1%TFA in ACN
 Gradient: 40-100% B in 20min, Flow rate: 1ml/min
 Column: Unitary C18, 4.6*150mm, 5um 100A
 Instrument: Agilent HPLC 1100
 Instrument: 1100
 Injection date: 2022/5/17 9:45:31
 Last changed: 2022/5/17 11:07:01
 Location: 2
 Injection: 1 of 1
 Injection volume: 5.000
 Acq. operator: SYSTEM

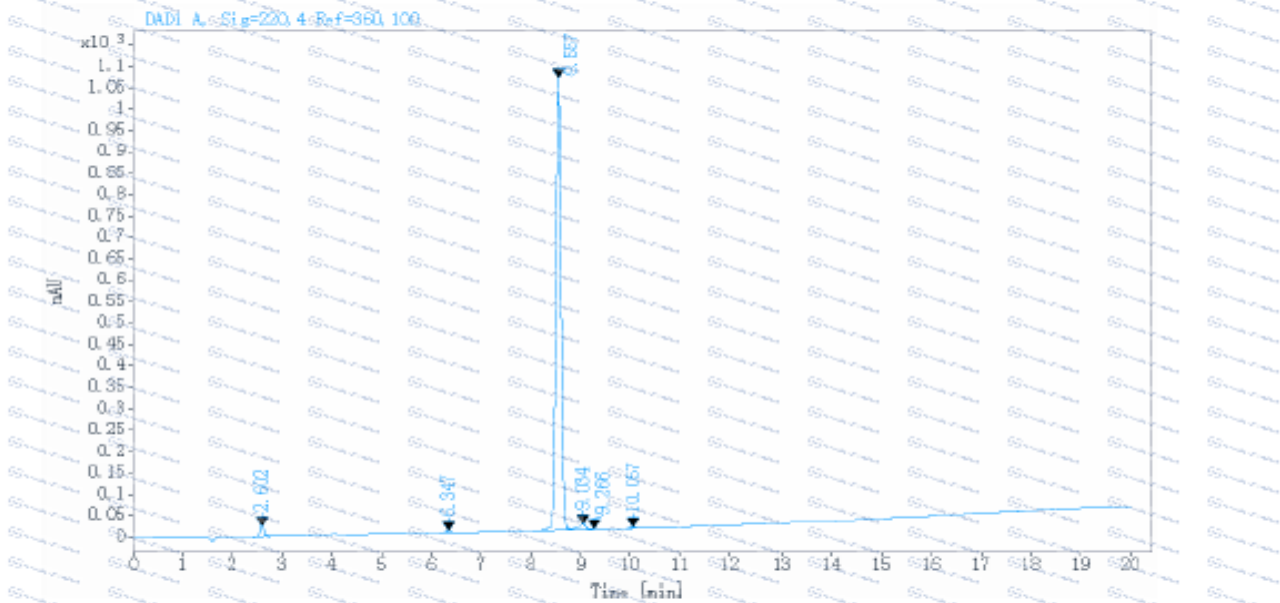

Signal: DAD1 A, Sig=220.4 Ref=360.100

| RT[min] | Type | Width[min] | Area | Height | Area% | Name |
|---------|------|------------|-----------|-----------|---------|------|
| 2.602 | BB | 0.1076 | 143.3130 | 24.7514 | 1.8987 | |
| 6.347 | BB | 0.1237 | 25.1780 | 3.5075 | 0.3336 | |
| 8.557 | BV F | 0.1218 | 7190.2642 | 1025.5020 | 95.2595 | |
| 9.034 | VV E | 0.1774 | 148.3688 | 12.5947 | 1.9656 | |
| 9.266 | VV E | 0.1382 | 16.8123 | 1.8477 | 0.2227 | |
| 10.057 | BB | 0.1123 | 24.1421 | 3.5056 | 0.3198 | |
| | Sum | | 7548.0783 | | | |

*For laboratory or manufacturing use only, not for drug, food and household use.

*If you have any comments and suggestions, please contact us by sales@amadischem.com