


## HPLC of 5522-66-7

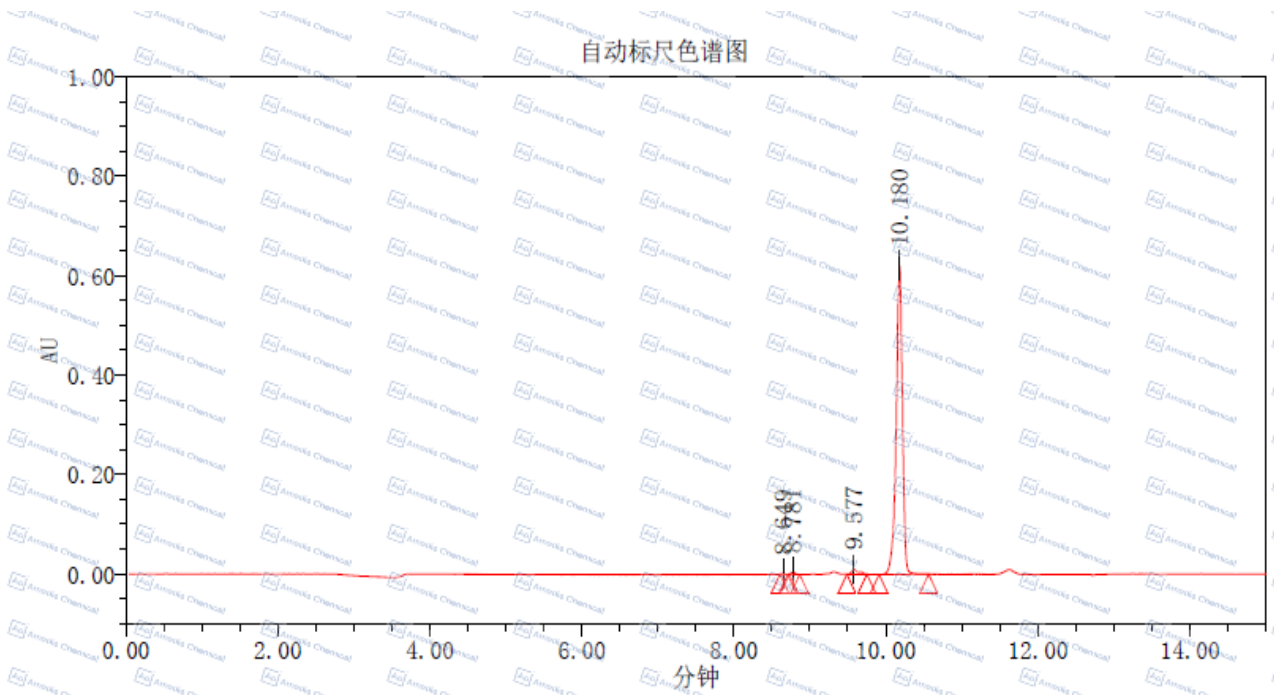

峰结果

名称	保留时间 (分钟)	面积 (微伏*秒)	高度 (微伏)	% 面积	USP 分离度	USP 理论塔板数	USP 拖尾
1	8.649	4116	1758	0.11			
2	8.781	14182	4941	0.39			
3	9.577	60716	10314	1.66			
4	10.180	3572381	621437	97.84			

\*For laboratory or manufacturing use only, not for drug, food and household use.

\*If you have any comments and suggestions, please contact us by [sales@amadischem.com](mailto:sales@amadischem.com)