


HPLC OF 1418013-75-8

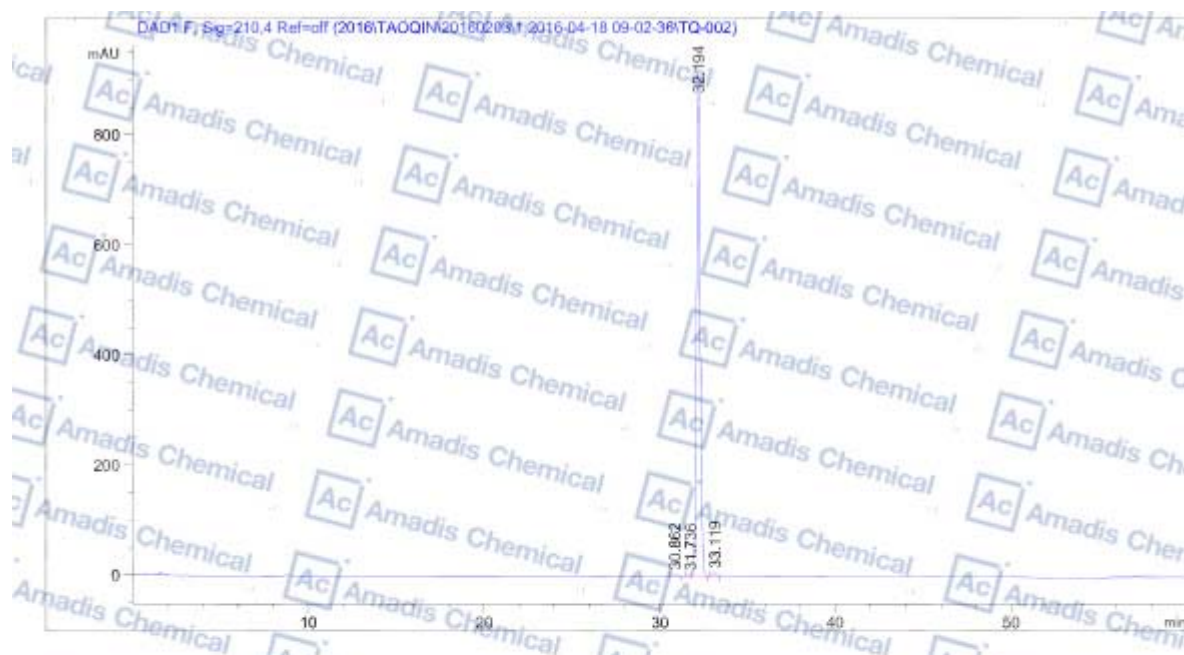

Area Percent Report

Sorted By : Signal
 Multiplier : 1.0000
 Dilution : 1.0000
 Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 F, Sig=210,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area
1	30.862	MF	0.2363	44.83726	3.16296	0.3381
2	31.736	MF	0.2375	22.78434	2.06097	0.1718
3	32.194	FM	0.2375	1.34090e4	920.01294	98.8574
4	33.119	MF	0.2333	83.89628	5.99266	0.6327
5	33.26054	MF	0.2333	931.22954	931.22954	98.8574

* If you have any comments and suggestions, please contact us by sales@amadischem.com