


HPLC Of 81846-19-7

Sample Name: UT15	Acquired By: 1120
Sample Type: Unknown	System: HPLC00
Batch No. 1/E_3	Sample Set Name: 20160315_HPLC003
Vial: 1	Sample Set Method: 20160315_HPLC003
Injection #: 1	Acq. Method Set: UT15
Injection Volume: 10.00 ul	Instrument Method Name: UT15
Injection Id: 1120	Instrument Method Id: UT15
Run Time: 70.0 Minutes	Processing Method: 00
Date Acquired: 03/15/2016 7:36:10 PM CST	Processing Method Id: UT15_20
Date Processed: 03/15/2016 8:51:44 AM CST	Channel Description: DAD VL AU Ch 1 Sample 217, BW 4
Column_ID: LC-38	

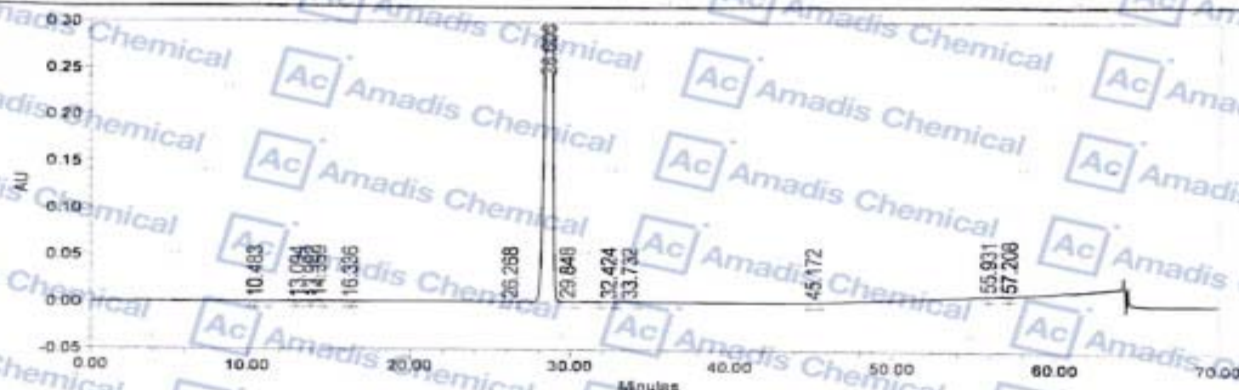

RT	Area	% Area	RT	Area	% Area
1 10.483	2745	0.015	11 45.172	2381	0.013
2 13.094	992	0.005	12 55.931	3427	0.018
3 13.992	1973	0.010	13 57.208	2024	0.011
4 14.389	7669	0.041			
5 16.336	1070	0.006			
6 28.268	3460	0.018			
7 28.806	18882030	99.780			
8 29.846	7539	0.040			
9 32.424	2000	0.011			
10 33.732	6405	0.034			

Reported by User: 1120

Report Method: ARD Individual Report

Report Method ID: 3429

Page: 1 of 1

Project Name: UT15

Date Printed:

03/15/2016

14:14:57 AM PRC

* If you have any comments and suggestions, please contact us by sales@amadischem.com