


HPLC Of 433289-83-9

实验时间: 2017-06-13, 9:24:06

实验者: 报告时间: 2017-06-13, 9:39:50

Chromatogram (VATS-EP-A.ora)

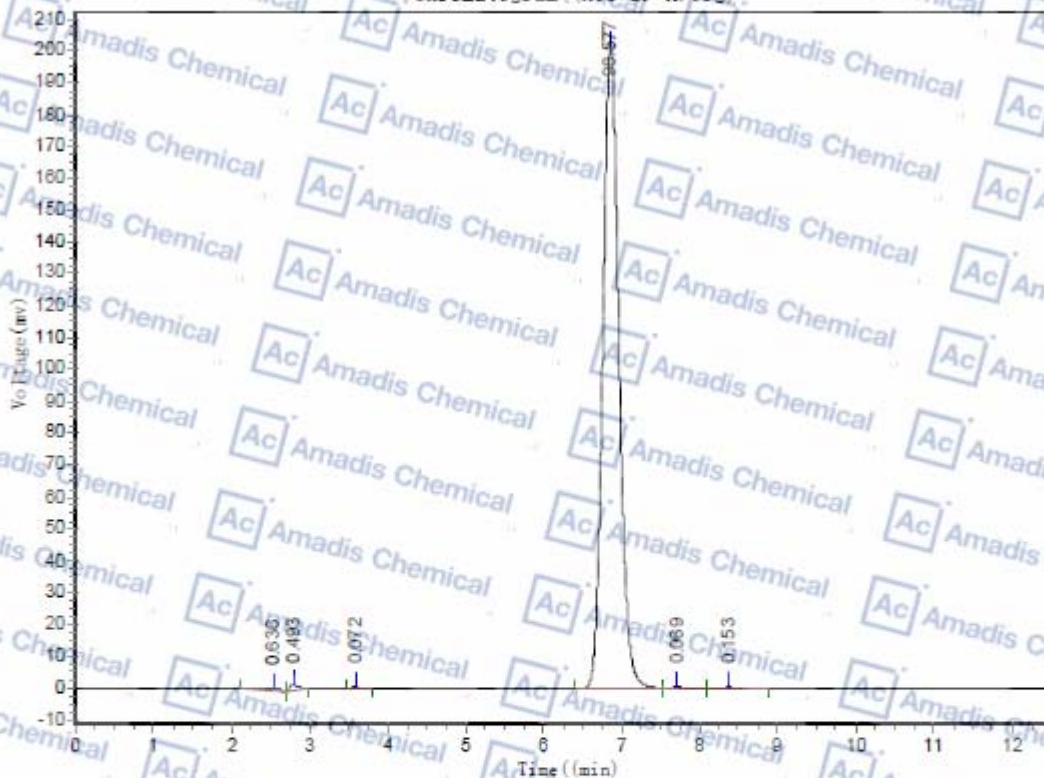

Results Table of the Analysis

Peak#	Name	Retime	Height	Area	Area (%)
1		2.540	1114.433	18581.850	0.6364
2		2.790	1966.806	14396.900	0.4931
3		3.582	301.571	2094.100	0.0717
4		6.857	201640.734	2878279.000	98.8774
5		7.715	163.136	2006.900	0.0687
6		8.365	266.853	4458.950	0.1527
Totals:			205452.533	2919817.700	100.0000

Peak Parameter Table

Width	Slope	Drift	Min Area	Variable	Locking	Stop	Sample weight
5	70.000	0.000	1000.000	0.000	0.000	12.538	100.0000

* If you have any comments and suggestions, please contact us by sales@amadischem.com