


HPLC of 2314-37-6

实验条件

填料: SinoChrom ODS-EP 5 μ m	流速: 1.0 mL/min
流动相: ACN: H ₂ O (TFA)	检测器: UV 254 nm
柱长: 200 mm	进样量: 5 μ L
柱径: 4.6 mm	

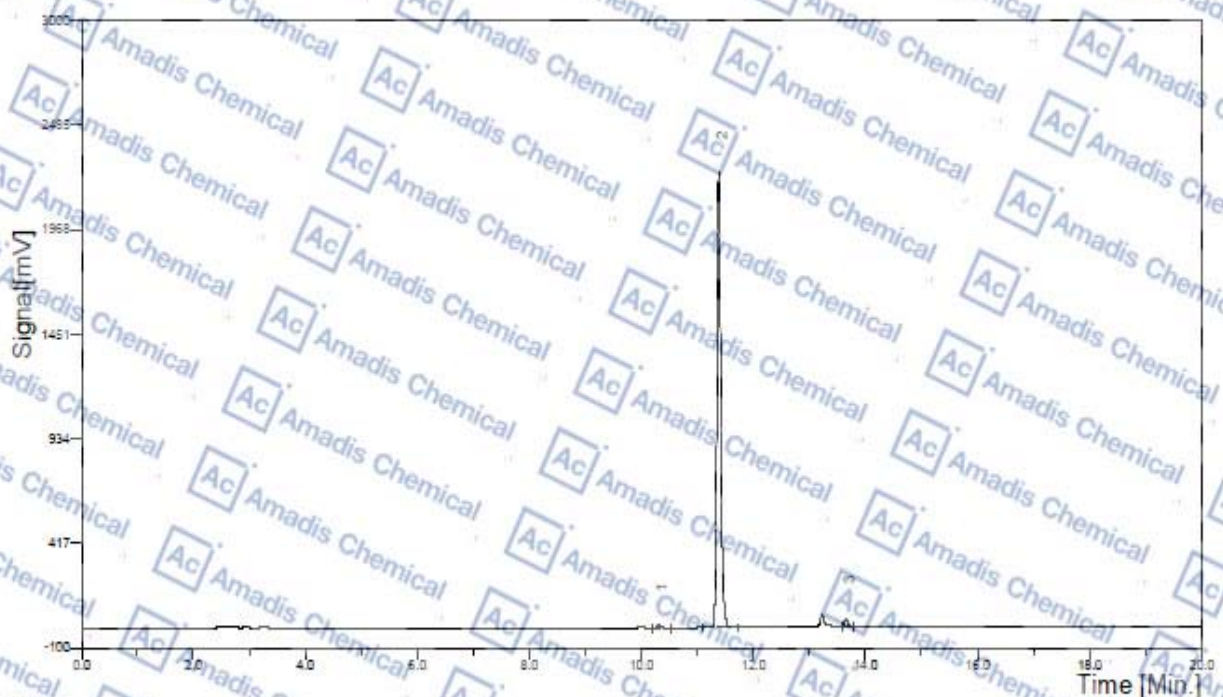

组分表

#	组分名	保留时间 (min)	峰高 (mV)	峰面积 (mV.sec)	面积百分比 (%)	浓度	样品含量 (%)
1	Unknown	10.30750	10.95	44.14	0.4245	0.0000	0.0000
2	Unknown	11.37917	2246.13	10181.00	97.9290	0.0000	0.0000
3	Unknown	13.65250	11.33	171.16	1.6464	0.0000	100.0000
合计			2298.41	10396.30	100		

* If you have any comments and suggestions, please contact us by sales@amadischem.com