


HPLC of 154737-89-0

Sample ID : WX00029-33
 Compound ID : 33
 Data File : D:\DATA\2017\201705\20170508-5\WX00029-33.D
 Acq. Method : D:\DATA\2017\201705\20170508-5\0-60AA_14MIN 1.M
 Column : Agilent Ecilpse Plus C18 3.5µm, 4.6*100mm
 Inj. time : 2017-05-08 14:54:58
 Inj. Volume : 1.00
 Inj. Location : P2-G-01
 Instrument : HPLC G
 Operator : LY Juan

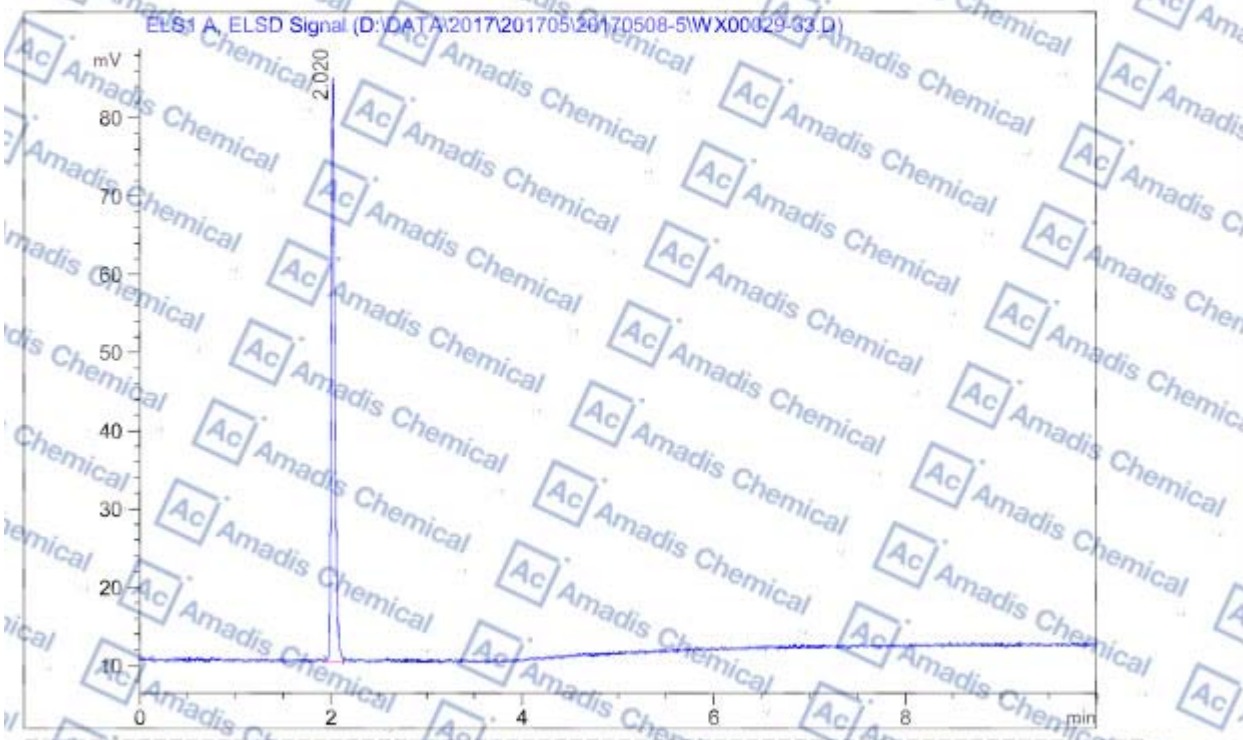

Signal	Meas.	Ret. Tim	Height	Area	Area %
ELS1 A, ELSD Signal	1	2.020	74.327	193.086	100.000

* If you have any comments and suggestions, please contact us by sales@amadischem.com