


### HPLC of 4359-87-9

Acq. Operator : Seq. Line : 2  
 Acq. Instrument : instrument 1 Location : Vial 13  
 Injection Date : 9/12/2013 11:10:42 AM Inj : 1  
 Inj Volume : 0.2 µl  
 Acq. Method : C:\Chem32\1\DATA\CF0164\20130912-RK 2013-09-12 10-41-18\503-CZ-RK.M  
 Last changed : 9/12/2013 10:41:16 AM  
 Analysis Method : C:\CHEM32\1\METHODS\503-CZ-RK.M  
 Last changed : 9/12/2013 12:30:02 PM  
 (modified after loading)  
 Method Info : Instrument:Agilent 1100HPLC  
 Column:Benepach C18 250\*4.6, 5µm  
 Mobile phase:B-Acetonitrile A=0.1%TFA  
 Gradient:5%-95%B in 12 min,95%B in isocratic for 10 min  
 Flow rate:1.0ml/min  
 Column temperature:35

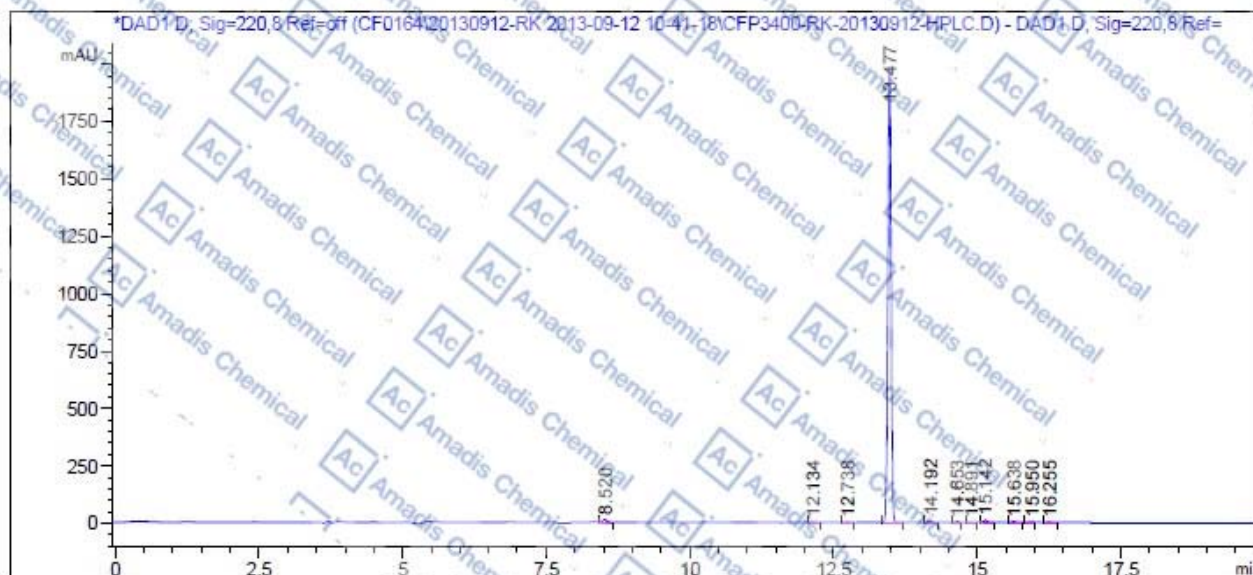

Area Percent Report

Sorted By : Signal  
 Multiplier : 1.0000  
 Dilution : 1.0000  
 Use Multiplier \* Dilution Factor with ISTDs

Signal 1: DAD1.D, Sig=220.8 Ref=off  
 Signal has been modified after loading from rawdata file!

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	8.520	BBA	0.0744	61.15313	12.21270	0.7573
2	12.134	BB	0.0664	13.98729	3.23660	0.0732
3	12.738	BB	0.0653	6.55918	1.55217	0.0812

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
4	13.477	BB	0.0622	7885.50537	1984.35071	97.3558
5	14.192	BB	0.0654	26.96775	6.35037	0.3332
6	14.653	BV	0.0558	13.91604	3.68299	0.1723
7	14.894	VB	0.0705	5.22044	1.11738	0.0646
8	15.142	BB	0.0676	39.84064	9.09913	0.4934
9	15.638	BB	0.0690	20.93358	4.44245	0.2592
10	15.950	BV	0.0707	16.19030	3.33223	0.2005
11	16.255	VB	0.0987	8.81506	1.30616	0.1092
Totals :				8075.02875	2030.79280	

\* if you have any comments and suggestions, please contact us by [sales@amadischem.com](mailto:sales@amadischem.com)