


HPLC of 92525-10-5

Acq. Operator : 1
Acq. Instrument : Instrument 1 Location : Vial 0
Injection Date : 7/4/2014 1:20:24 PM
Acq. Method : D:\CHEM32\
Last changed : 12/9/2013 8:15:27 PM by 1
Analysis Method : D:\CHEM32\
Last changed : 7/4/2014 1:31:32 PM by 1
(modified after loading)
Sample Info : A = ACN, B = 0.1% H3PO4/H2O 10-95% A/B 3.5 min, 95% A/
B 4.5 min, 95-10% A/B 1 min, 10% A/B 1 min; Athena C18
(3 µm, 2.1 mm × 100 mm); Flow: 0.4 ml/min

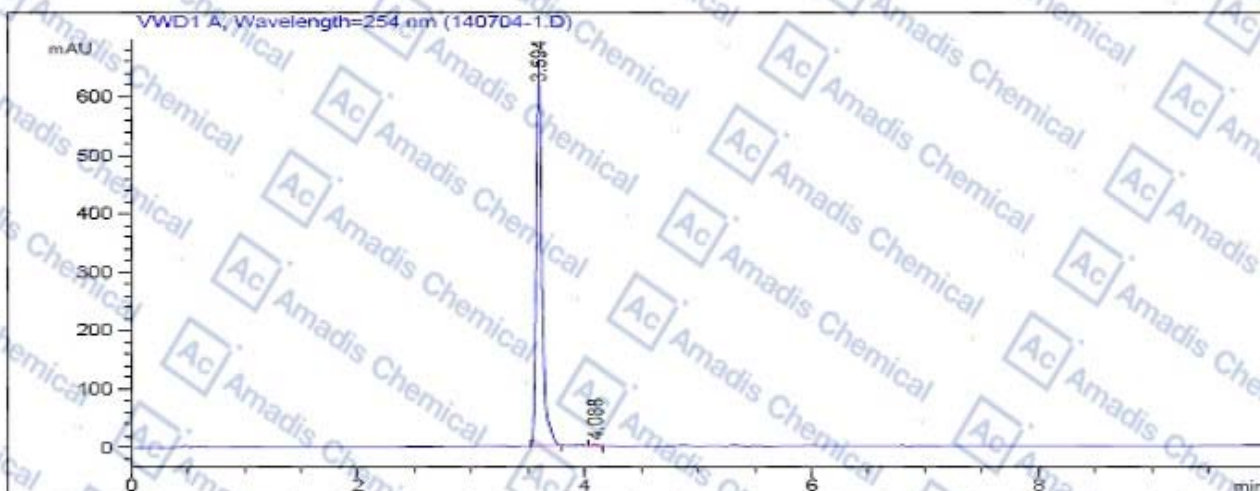

Area Percent Report

Sorted By : Signal
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs
Signal 1: VWD1 A, Wavelength=254 nm

* If you have any comments and suggestions, please contact us by sales@amadischem.com