
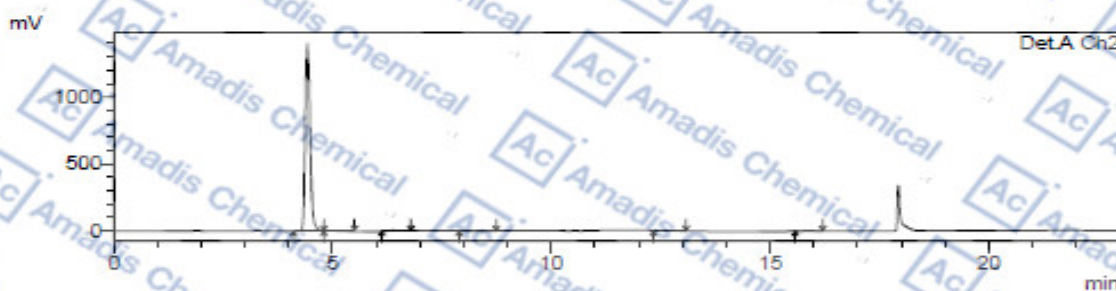


HPLC of 415903-37-6

Column : Inertil ODS-3, 5um 4.6*150mm
 Mobile phase : Solvent A: H2O(0.05%H3PO4) Solvent B:ACN(0.05%H3PO4)
 Temperature : 40 °C
 Flow rate : 1mL/min
 Run time : 3min gradient(20%B), 12min gradient (20%-50%B), 5min gradient (50%-95%B),3 min(95%B),th
 Detector : UV
 Wavelength : 220/254 nm
 User name : 415903-37-6
 Notebook page :
 Sample description : 1mg/ml in ACN
 Injection Volume : 3 uL
 Data File Name : 415903-37-6.lcd
 Method File Name : 415903-37-6.lcm
 Batch File Name : 20171021.lcb
 Data Acquired : 2017-10-21 9:20:39
 Data Processed : 2017-10-21 10:47:59

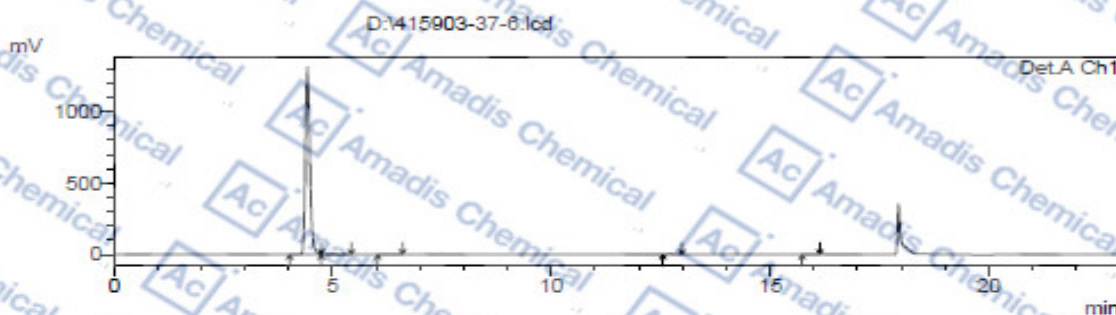

1:Det.A Ch1/220nm
 2:Det.A Ch2/254nm

Peak Table

Peak#	Ret. Time	Area	Area %	Theoretical Plates
1	4.419	9293696	99.355	8183.204
2	4.750	26707	0.286	0.000
3	6.384	10066	0.108	16246.620
4	12.711	14512	0.155	61468.853

Peak#	Ret. Time	Area	Area %	Theoretical Plate
5	15.873	9074	0.097	57418.505
Total		9354055	100.000	

PeakTable

Detector A Ch2 254nm

Peak#	Ret. Time	Area	Area %	Theoretical Plate
1	4.419	10644823	99.136	7208.014
2	4.855	26678	0.248	1444.129
3	6.382	30127	0.281	14424.852
4	8.287	12437	0.116	18670.204
5	12.713	13545	0.126	52027.509
6	15.875	10002	0.093	52132.873
Total		10737612	100.000	

*If you have any comments and suggestions, please contact us by sales@amadischem.com