


HPLC of 1229705-06-9

Column : Inertil ODS-3, 5um 4.6*150mm
 Mobile phase : Solvent A: H2O(0.05%H3PO4) Solvent B:ACN(0.05%H3PO4)
 Temperature : 40 °C
 Flow rate : 1mL/min
 Run time : 3min gradient(90%B), 15min gradient (90%-95%B),5 min(95%B),then 7min @90%B)
 Detector : UV
 Wavelength : 220/254 nm
 User name : ZJB E-005
 Notebook page :
 Sample description : in ACN
 Injection Volume : 4 uL

Data File Name : 1229705-06-9.lcd
 Method File Name : 1229705-06-9.lcm
 Batch File Name : 20170428.lcb
 Data Acquired : 2017-5-2 11:55:48
 Data Processed : 2017-5-2 12:59:31

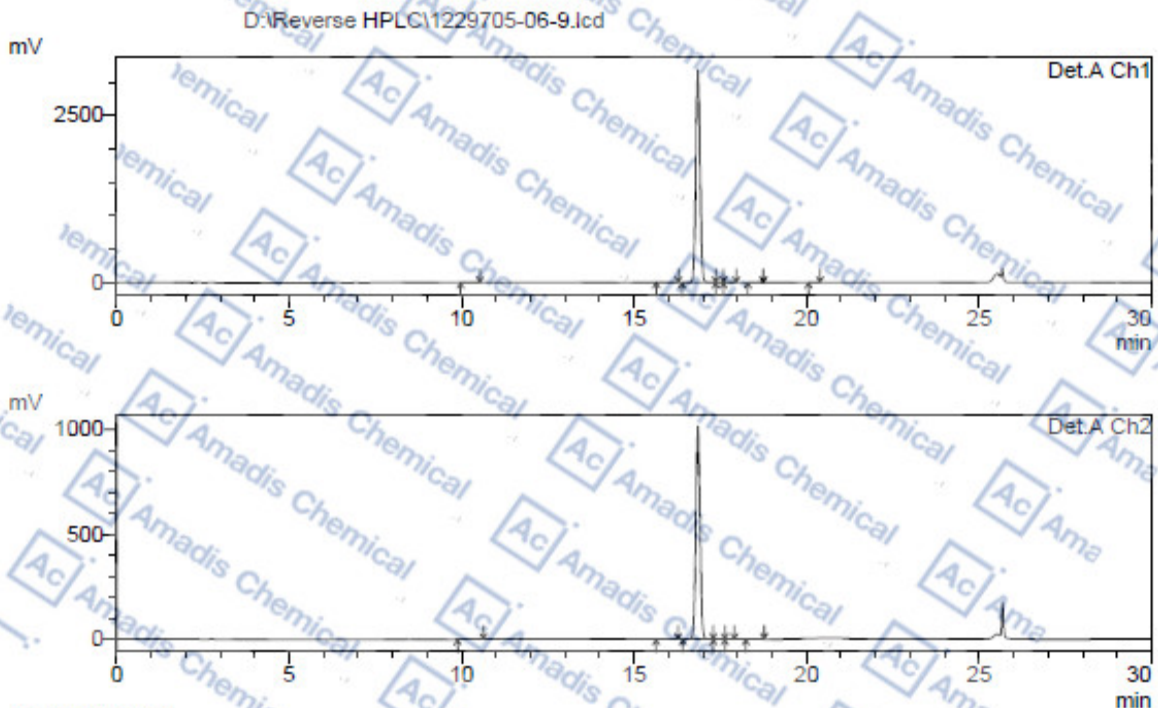

PeakTable

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Area %	theoretical Plates
1	10.270	5177	0.019	29117.439
2	15.968	21070	0.077	56864.873
3	16.848	27302262	99.744	81232.112
4	17.426	11369	0.042	65459.595

Peak#	Ret. Time	Area	Area %	Theoretical Plates
5	17.721	14949	0.055	67963.985
6	18.531	4849	0.018	93313.359
7	20.222	12544	0.046	102934.798
Total		27372219	100.000	

PeakTable

Detector A Ch2 254nm

Peak#	Ret. Time	Area	Area %	Theoretical Plates
1	10.267	7438	0.085	29538.046
2	15.968	8384	0.096	57243.475
3	16.848	8722819	99.601	81107.574
4	17.424	5015	0.057	61940.136
5	17.716	3889	0.044	78585.016
6	18.532	10233	0.117	76721.513
Total		8757778	100.000	

* If you have any comments and suggestions, please contact us by sales@amadischem.com