


HPLC of 926927-61-9

SAMPLE INFORMATION

Sample Name:	VTX-2337	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	1	Acq. Method Set:	Gradient 30 to 100 in 10min
Injection #:	1	Processing Method:	12
Injection Volume:	10.00 µl	Channel Name:	2487Channel 1
Run Time:	15.0 Minutes	Proc. Chnl. Descr.:	254nm
Date Acquired:	2017-12-27 19:29:52 CST		
Date Processed:	2018-2-5 15:50:56 CST		

Auto-Scaled Chromatogram

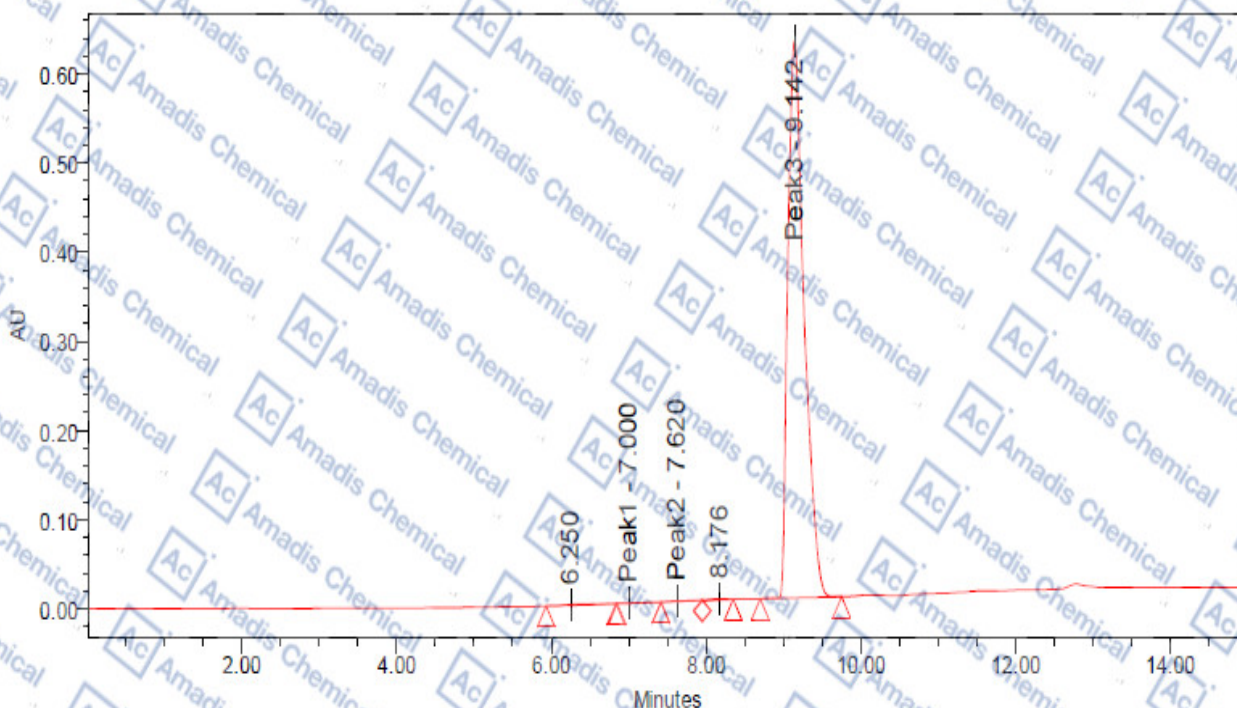

Peak Results

	RT	Area	Height	Width (sec)	% Area
1	6.250	15028	742	54.000	0.16
2	7.000	1619	127	34.000	0.02
3	7.620	12554	799	32.000	0.14
4	8.176	12338	1087	24.000	0.13
5	9.142	9123639	626854	63.000	99.55

* If you have any comments and suggestions, please contact us by sales@amadischem.com