


## HPLC of 214766-78-6

**Data file:** E:\DATA\180805\800064 18070022Final.D  
**Sample name:** 800064 18070022Final  
**Description:** Mobile phase: Buffer A:0.1%TFA in H2O Buffer B:0.1%TFA in ACN  
 Gradient:30-40% in 25min, Flow rate:1.0ml/min  
 Column:Unitary C18, 4.6\*150mm, 5um 100A (A-001)  
 Instrument:Agilent HPLC 1100  
**Instrument:** QC **Location:** 52  
**Injection date:** 2018/8/5 13:55:07 **Injection:** 1 of 1  
**Last changed:** 2018/8/5 14:08:57 **Injection volume:** 5.000  
**Acq. operator:** QC\_1

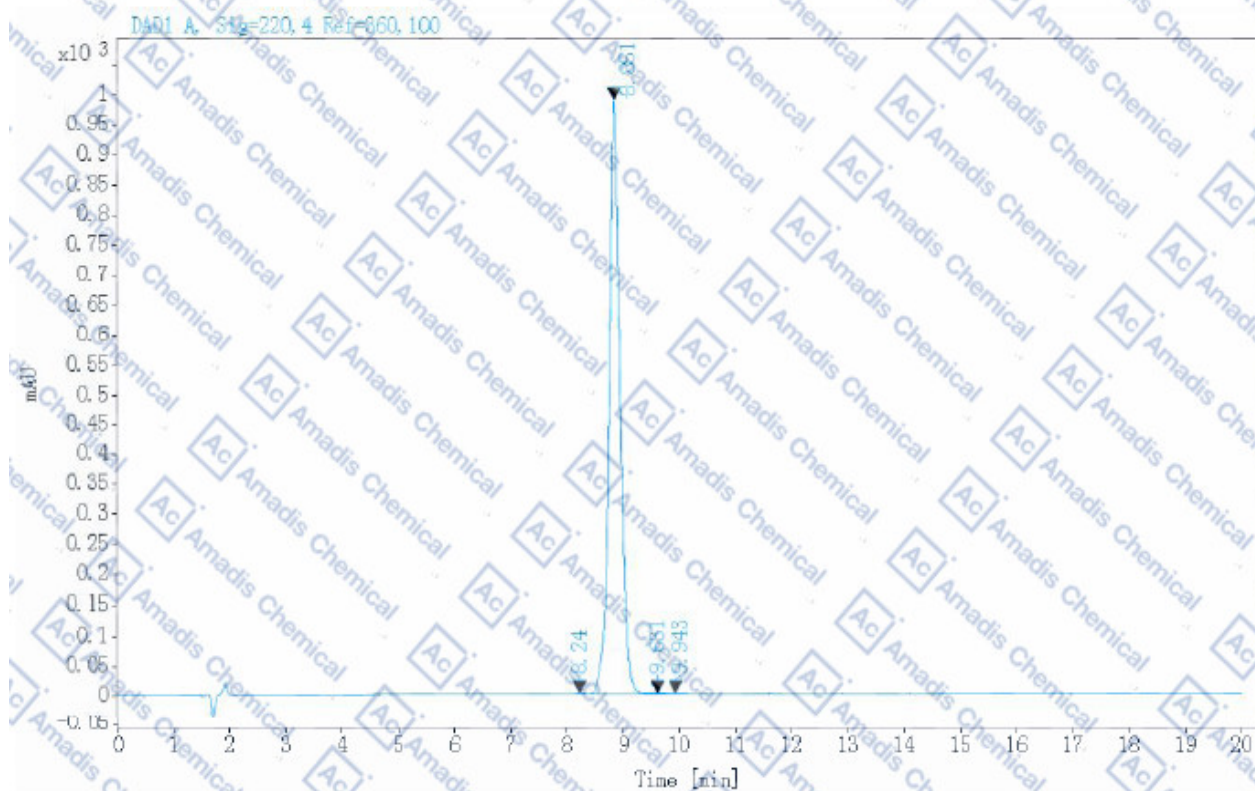

**Signal:** DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area%	Name
8.240	VV E	0.2532	27.8644	1.5839	0.2021	
8.851	VV R	0.2133	13689.5225	989.8796	99.2703	
9.631	VV E	0.2508	26.7350	1.5084	0.1939	
9.943	VV E	0.2529	46.0321	2.6208	0.3338	
	Sum		13790.1540			

\*If you have any comments and suggestions, please contact us by [sales@amadischem.com](mailto:sales@amadischem.com)