


## HPLC of 254750-02-2

HPLC REPORT			
Sample Name:	ES-P	Injection Volume:	10.0
Vial Number:	RD2	Channels:	UV_VIS_1
Sample Type:	unknown	Wavelength:	254
Control Program:		Bandwidth:	4
Quantif. Method:	default	Dilution Factor:	1.0000
		Sample Weight:	1.0000
Run Time (min):	15.13	Sample Amount:	1.0000

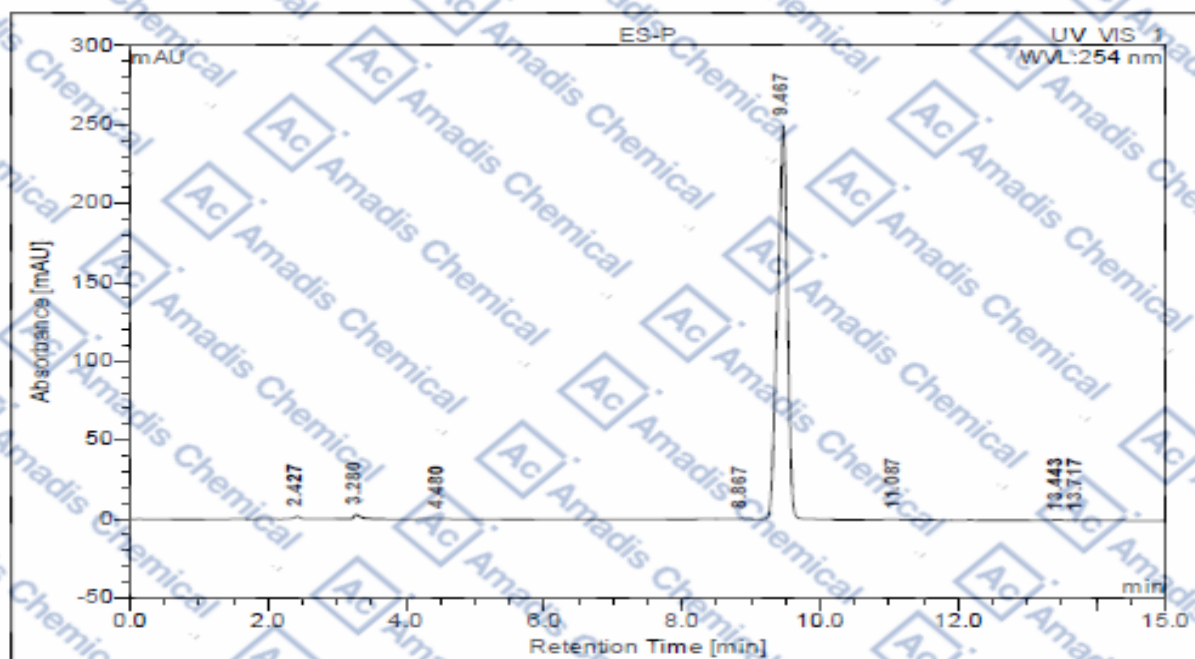

No.	Ret. Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount n.a.	Type
1	2.43	n.a.	1.663	0.186	0.44	n.a.	BMB*
2	3.28	n.a.	2.667	0.321	0.77	n.a.	BMB*
3	4.48	n.a.	0.251	0.068	0.16	n.a.	BMB*
4	8.87	n.a.	0.341	0.058	0.14	n.a.	BMB*
5	9.47	n.a.	249.407	41.087	98.01	n.a.	BMB*
6	11.09	n.a.	0.379	0.079	0.19	n.a.	BMB*
7	13.44	n.a.	0.249	0.096	0.23	n.a.	BM *
8	13.72	n.a.	0.151	0.028	0.07	n.a.	MB
<b>Total:</b>			255.108	41.922	100.00	0.000	

\*If you have any comments and suggestions, please contact us by [sales@amadischem.com](mailto:sales@amadischem.com)