

HPLC of 1229453-99-9


<Sample Information>

Sample Name : 445-P
 Data Filename : 445-P-LC1.lcd
 Batch Filename : 20190530.lcb
 Date Acquired : 5/30/2019 10:56:10 AM
 Date Processed : 5/30/2019 11:20:18 AM
 Method Filename : M-A90B10.lcm
 Vial # : 1-78
 Injection Volume : 0.2 uL
 Acquired by : System Administrator
 Processed by : System Administrator

SunFire C18 5um 4.6x150mm 25C 1.000ml/min 16min

<<Mobile Phase Name>>
 Mobile Phase B : 0.03%TFA in ACN
 Mobile Phase A : 0.03%TFA in H2O

<Chromatogram>

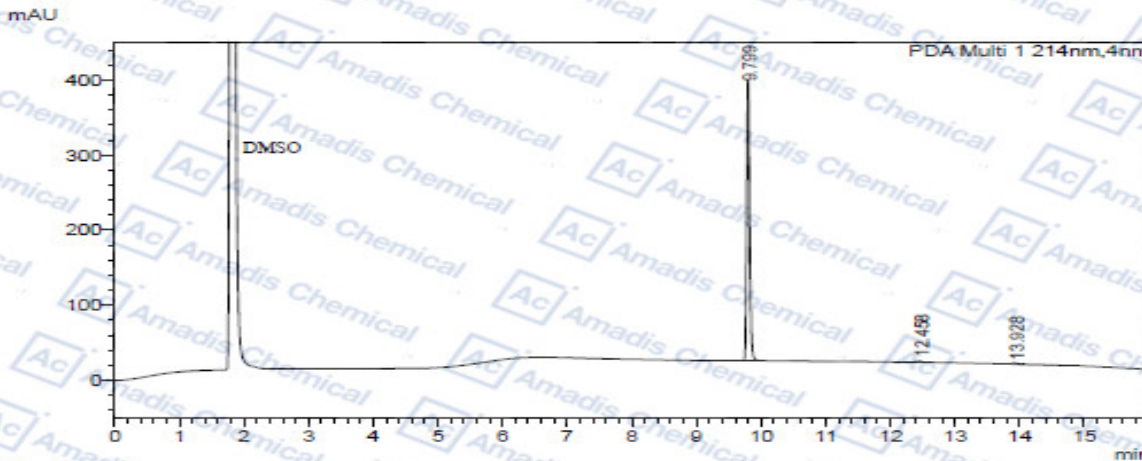

<Peak Table>

Peak#	Ret. Time	USP Width	Height	Area	S/N	Area%
1	9.799	0.091	374488	1176607	6.23	98.437
2	12.458	0.167	1793	10028	0.03	0.839
3	13.928	0.158	1534	8657	0.03	0.724
Total				1195292		100.000


<Sample Information>

Sample Name : 445-P
 Data Filename : 445-P-LC1.lcd
 Batch Filename : 20190530.lcb
 Date Acquired : 5/30/2019 10:56:10 AM
 Date Processed : 5/30/2019 11:21:05 AM
 Method Filename : M-A90B10.lcm
 Vial # : 1-78
 Injection Volume : 0.2 uL
 Acquired by : System Administrator
 Processed by : System Administrator

SunFire C18 5um 4.6x150mm 25C 1.000ml/min 16min

<<Mobile Phase Name>>
 Mobile Phase B : 0.03%TFA in ACN
 Mobile Phase A : 0.03%TFA in H2O

<Chromatogram>

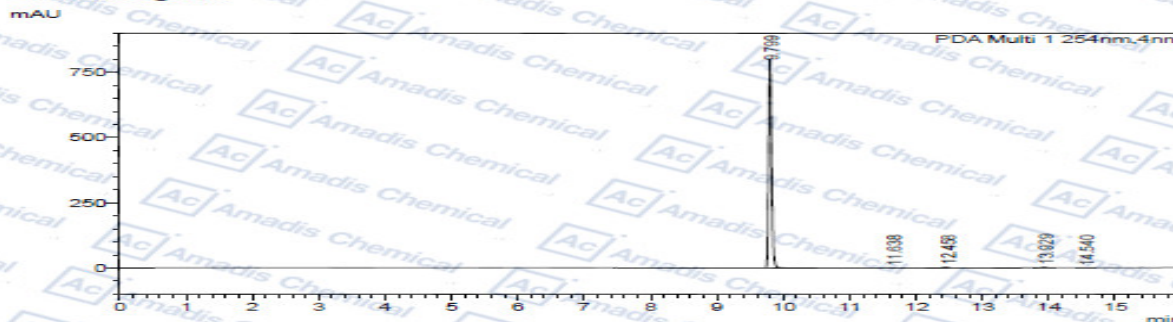

<Peak Table>

Peak#	Ret. Time	USP Width	Height	Area	S/N	Area%
1	9.799	0.091	800936	2525038	7674.81	98.167
2	11.638	0.288	281	3345	2.69	0.130
3	12.458	0.172	3656	20252	35.03	0.787
4	13.929	0.165	3301	20032	31.63	0.779
5	14.540	0.162	592	3530	5.67	0.137
Total				2572197		100.000

*if you have any comments and suggestions, please contact us by sales@amadischem.com