


## HPLC of 195514-23-9

### Chromatogram and Results

Injection Details		
Injection Name:	0410-01313	Run Time (min): 46.00
Vial Number:	GB3	Injection Volume: 2.00
Injection Type:	Unknown	Channel: UV_VIS_1
Calibration Level:		Wavelength: 214.0
Instrument Method:	GDL 0-30min ACN2%-90% with wash and baseline	Bandwidth: 4
Processing Method:	Processing Method	Dilution Factor: 1.0000
Injection Date/Time:	10/四月/19 12:34	Sample Weight: 1.0000

### Chromatogram

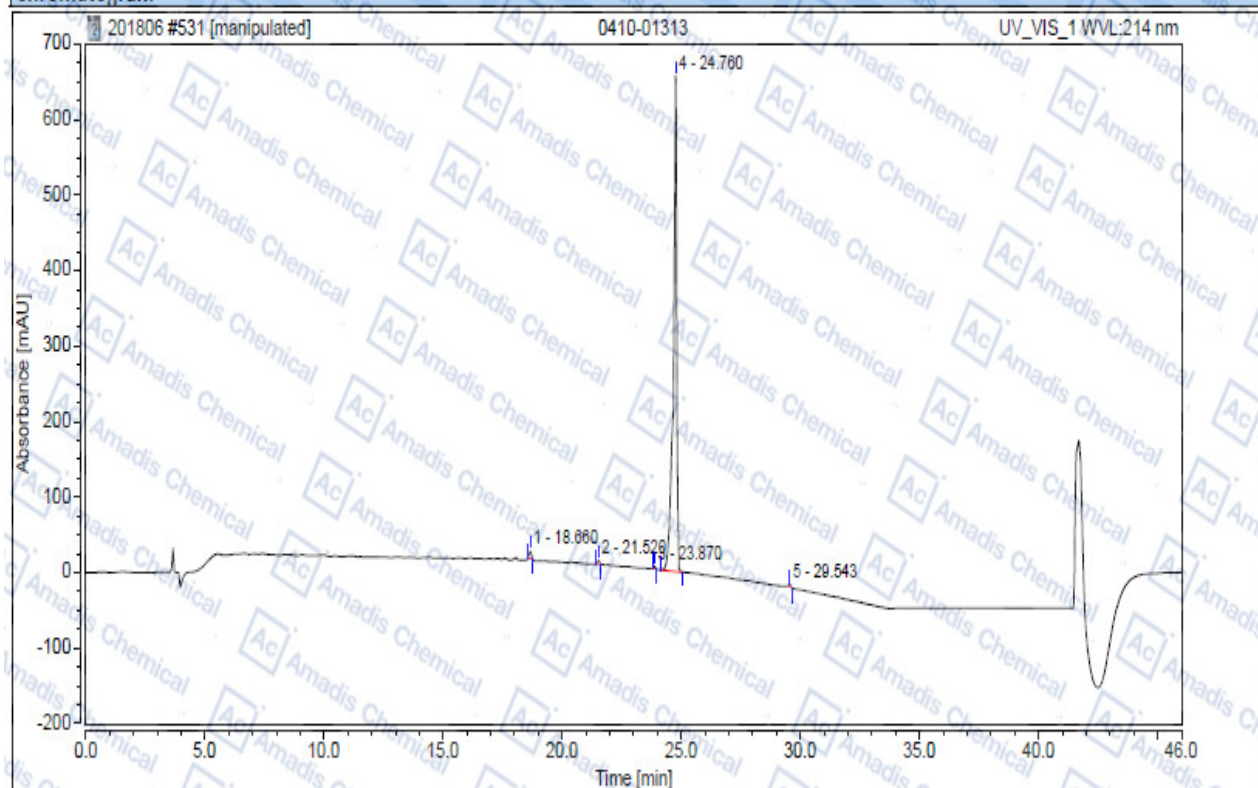

Integration Results							
No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount n.a.
1		18.660	1.107	10.187	1.02	1.50	n.a.
2		21.520	0.504	5.144	0.47	0.76	n.a.
3		23.870	0.247	3.215	0.23	0.47	n.a.
4		24.760	106.221	656.679	98.09	96.84	n.a.
5		29.543	0.210	2.854	0.19	0.42	n.a.
<b>Total:</b>			<b>108.289</b>	<b>678.078</b>	<b>100.00</b>	<b>100.00</b>	

\* if you have any comments and suggestions, please contact us by [sales@amadischem.com](mailto:sales@amadischem.com)